


Nichipet[®] Air

User's Manual

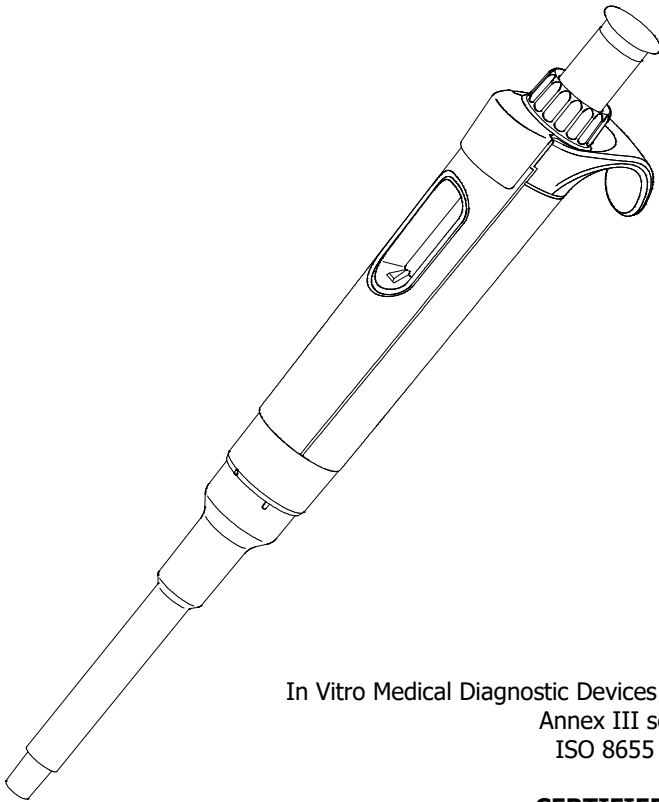

In Vitro Medical Diagnostic Devices (98/79/EC)
Annex III self-declared
ISO 8655 STANDARD

CERTIFIED ISO9001




FUTURE LIFESCIENCE PARTNER
NICHIRYO





Nichipet[®] Air

Thank you very much for purchasing Nichipet Air.
Please read this manual carefully before using this device.

Safety Precautions

- Please read this manual carefully and have sufficient understanding of the contents and instructions, especially concerning matters of safety, prior to use.
- The notes stated here is for the safety of the user, and for the correct usage of the product.
- After reading this manual, please keep it in a noticeable and accessible place for 'users of the device' to refer to at any time.

Danger Levels

 DANGER	Will lead to serious injuries or death.
 WARNING	May lead to severe injuries or death.
 CAUTION	May lead to light to moderate injuries, and/or cause property damage.
	User information

Caution on disposal of this product

When disposing the pipette body and tips (including adhering liquid), please comply with the laws and regulations of each country related to disposal, or local ordinance or regulation.

Nichipet[®] Air

Table of Contents

1. Product overview	3
1.1 Features	3
1.2 Standard accessories (Included)	3
1.3 Main illustration	4
2. Information on safety	4
2.1 Intended use	4
2.2 Material information	6
3. Operation/Operating procedure	6
3.1 Volume setting	6
3.2 Aspiration of liquid (Forward technique)	7
3.3 Dispensing the liquid	8
3.4 Recommendation for accurate pipetting (Technique)	9
4. Maintenance	10
4.1 Cleaning	10
4.1.1 Disassembling	10
4.1.2 Reassembling	12
4.1.3 Lubrication/Greasing	21
4.2 Autoclaving	22
4.2.1 Autoclave implementation procedure	22
4.2.2 Drying procedure	23
5. Specifications (Accuracy/Precision)	24
6. Calibration (Adjustments)	25
6.1 Volume adjustment method	25
6.2 Volume measurement/Inspection procedure	26
7. Troubleshooting	28
8. Replacement parts list	29
8.1 Consumables	29
8.2 Spare parts list	29

1. Product overview

1.1 Features


- The newly designed curvature and roundness in shape is ergonomic, and mitigates the user's fatigue and stress levels from long periods of use.
- Fully autoclavable at the condition of 121°C for 20 minutes.
- Eight types can be used for a wide range of sampling, from 0.1µL to 10,000µL. In addition, the volume sizes are indicated by colors, 2µL-gray, 10µL-pink, 20µL-cream, 100µL-orange, 200µL-yellow, 1000µL-blue, 5000µL-green, 10000µL-white. Since each type is displayed in a different color, they are easily identifiable.
- The body's hermetic part/airtight part uses high-performance and high-heat-resistant grease, thus maintaining excellent accuracy and precision, even when used over long periods of time.
- The special design and structure, makes it easy and intuitive to calibrate.

1.2 Standard accessories (Included)

Accessories	QTY
Tip (2µL, 10µL, 20µL, 100µL, 200µL, 1000µL,)	3
Tip (5000µL,10000µL)	1
Grease	1
Nozzle filter (5000µL,10000µL)	3
User's Manual	1

When unboxing the package, check that all of the items above are included for the respective model.

1.3 Main illustration

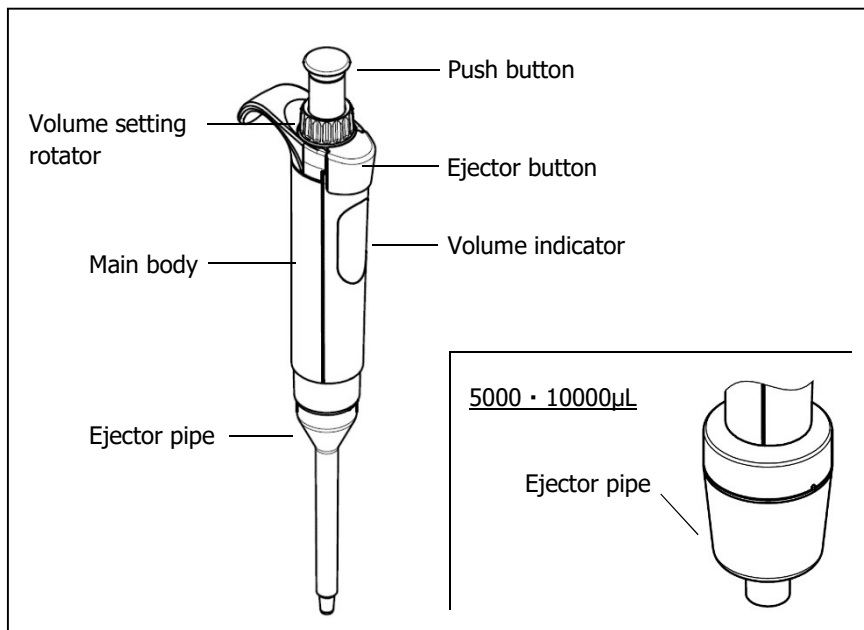

2. Information on safety

2.1 Intended use

Nichipet Air, used in conjunction with pipette tips recommended by Nichiryō, are designed and constructed for low-contamination transfer of liquids, especially for samples from the human body and for reagents within the scope of an in-vitro diagnostic application in order to allow the in-vitro diagnostic medical device to be used as intended.

Therefore, Nichipet Air is subjected to the accessories of in-vitro diagnostic medical devices under Directive 98/79/EC. The accessories is treated as in vitro diagnostic medical devices in their own right under Directive 98/79/EC.

Nichipet Air are intended for operation by qualified staff.

 DANGER

- ✓ When handling radioactive substances or infectious substances, always check and confirm the information first, and follow guidelines on their safety procedures.
 - ✓ When using harmful liquids to the human body, be very careful in the handling of the substances.
 - ✓ Never touch or come into direct contact with the used chips.
 - ✓ When liquids that are harmful to the human body adheres and/or contamination occurs, use appropriate measures to clean and decontaminate the device before continuing its use.
 - ✓ This product is not intended for use on living organisms.
 - ✓ Do not eject the tip with liquid inside of it.
 - ✓ Do not eject the tip towards anybody.
 - ✓ Do not expel or dispense any liquids towards anybody.
 - ✓ Depending on the splashed liquid, there is danger of causing injuries to the human body.
-

 WARNING

- ✓ Please protect yourself in accordance with the general procedure of danger prevention, such as wearing protective clothing, protective glasses and gloves.
-

 CAUTION

- ✓ Do not use the pipette for any other purpose, use only for pipetting and liquid dispensing.
 - ✓ Do not modify the pipette, modification can lead to accidents.
 - ✓ Do not stab the tip into the human body, or eject the tip towards anyone. The tip is very sharp and extremely dangerous.
 - ✓ Since the main body of the pipette becomes extremely hot right after autoclaving and drying. In this state, please do not touch it directly with your hands. It can lead to accidents and burn injury.
 - ✓ Do not use the pipette for any purpose other than pipetting and liquid dispensing, such as stirring liquid with this product. It can lead to loosening of the tip, the tip dropping off, liquid adhesion and contamination to the main unit of the device and accidents and/or injury.
-

2.2 Material information


CAUTION

- ✓ The use of highly reactive chemicals may damage the device. Please acknowledge the following materials that are used, and do not use liquids that will violate them.

Material of external parts

- Polypropylene (PP)
 - modified- Polyphenyleneether (m-PPE)
 - Polyetheretherketone (PEEK)
 - Fluororubber (FKM)
 - Stainless steel
 - Aluminum alloy
 - Polysulfone (PSU)
 - Polyphenylenesulfide (PPS)
-

3. Operation/Operating procedure


-  ✓ Do not expose pipette to direct sunlight when using it, or for 2 hours prior to use, otherwise the pipette may lose its accuracy. Avoid working with pipettes in a high temperature, low temperature, low humidity environment, or when the temperature difference between the environment including the main body of the device and the liquid is large, accuracy and precision may not be guaranteed.
 - ✓ Just prior to use, avoid touching the tip or nozzle cylinder as much as possible. If they are warmed up, accuracy may not be obtained.
 - ✓ Original Nichiryo tips are recommended. Nichipet Air is calibrated with the original Nichiryo tip, if you use other tips, deviations in original factory settings may occur, and accuracy will not be guaranteed.
-

3.1 Volume setting

- 1) Turn the volume setting rotator to set the volume indicator to a desired liquid volume. When setting the liquid volume, set the indicator's minimum graduation scale to the triangle point marker in the lower part of the volume indicator (Fig.A). Please refer to the volume indicator and the minimum graduation unit for each model to set the measurement volume accordingly. The volume indicator numbers are colored in black, or in red, to indicate the position of the decimal point. Black indicates the integer, red indicates the decimal. Scale units are in (μL).
- 2) To increase the volume setting, turn the volume setting rotator till it passes the designated volume setting by at least half a rotation of the rotator, and then dial back to set the designated volume.
- 3) To decrease the volume setting, simply turn it to the designated volume directly. (Fig. A)

⚠ CAUTION

- ✓ Do not exceed the specified liquid volume limit, otherwise the pipette may be damaged or deteriorate in its quality.

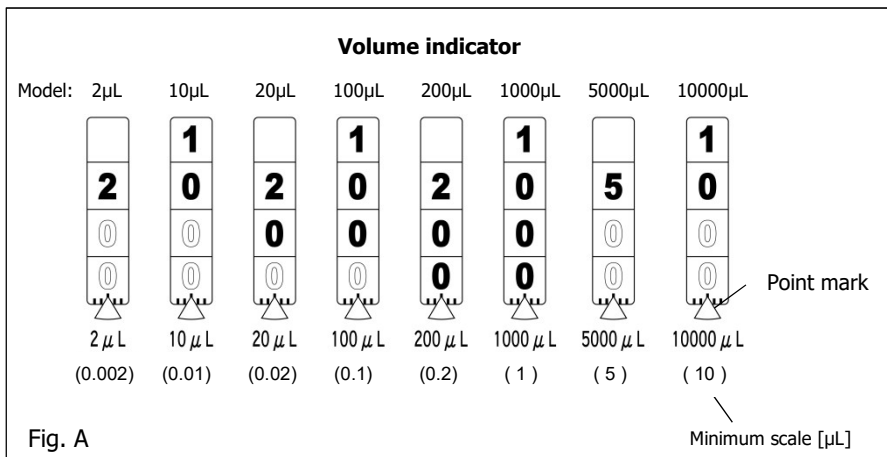

3.2 Aspiration of liquid (Forward technique)

- 1) Attach a new tip to the nozzle end.



- ✓ It is recommended that tips are directly picked up from the rack. Do not twist the pipette when fixing tip on.
- ✓ Please be sure to mount the tip on the main nozzle securely. Failure to do so may cause the tip to drop off and liquid to splash.

⚠ CAUTION

- ✓ Do not perform pipetting with less liquid than the set volume. If the quantity of liquid is less than the set volume, it may cause the liquid to spray into the main body, and the pipette may be damaged or deteriorate in its quality.

- 2) Press down the push button fully to the '1st stop'.
- 3) Hold the pipette vertically and immerse the tip 2mm. to 3mm. below the surface of the liquid (Fig. B) - ①.
- 4) To aspirate the set volume of liquid into the tip, release the push button slowly and let the push button go back to the initial position naturally. It takes 1 second to aspirate the liquid. During this operation, stop to wait for the suction process of the liquid to be totally completed, making sure that the liquid is drawn up into the tip with certainty (Fig. B) - ②.
- 5) Draw the tip of the pipette carefully vertically upward and away from the liquid surface, then touch the tip to the side of the tube to remove excess droplet adhering to the outside of the tip (Fig. B) - ③.



- ✓ Do not aspirate when the push button is at '2nd position' (Fig. B).
 - ✓ We recommend using the forward technique as the operation method of this device for pipetting. Nichipet Air has been calibrated with the forward method, and precision may not be obtained when dispensing by any other means.
 - ✓ Always change the tip when using different liquids to avoid cross-contamination.
-



CAUTION

- ✓ Please operate the push button slowly and gently. Sudden release of the push button, can lead to the aspiration of the liquid into the nozzle cylinder; not only precise accuracy will not be obtained, but also the quality of the device will be impaired.
 - ✓ When using the pipette, be sure to always attach and use a tip. Failure to do so, will lead to liquid entering the inside of the device's nozzle cylinder and cause serious malfunctions
 - ✓ Never turn the device sideways or upside down with liquid in the tip. Liquid can enter inside the device's nozzle cylinder, which can cause *contamination and breakdown.
-


*Cross-contamination with the entered liquid remaining inside the main body of the device can also occur, when switching liquids thereafter.

3.3 Dispensing the liquid

- 1) Touch the end of the tip against the inside wall of the recipient tube at a slight angle.
 - 2) Press the push button down slowly and smoothly to the '1st stop'.
Wait for a second, then press the push button down to the '2nd stop' to expel the last droplet of liquid from the tip (Fig. B) - ④ and ⑤.
 - 3) Keep the push button compressed. Remove the last droplet by slightly touching and running the end of the tip up against the inner wall of the tube, then move the tip of the pipette vertically straight up and out of the tube.
 - 4) Press the ejector button to detach the tip to dispose (Fig. B) – ⑥.
-



- ✓ We recommend the tip to be disposed of after each use. Repeated use may lead to and result in; loss of accuracy, precision, and may lead to contamination/cross-contamination due to adhesion and deposits from prior use.
-

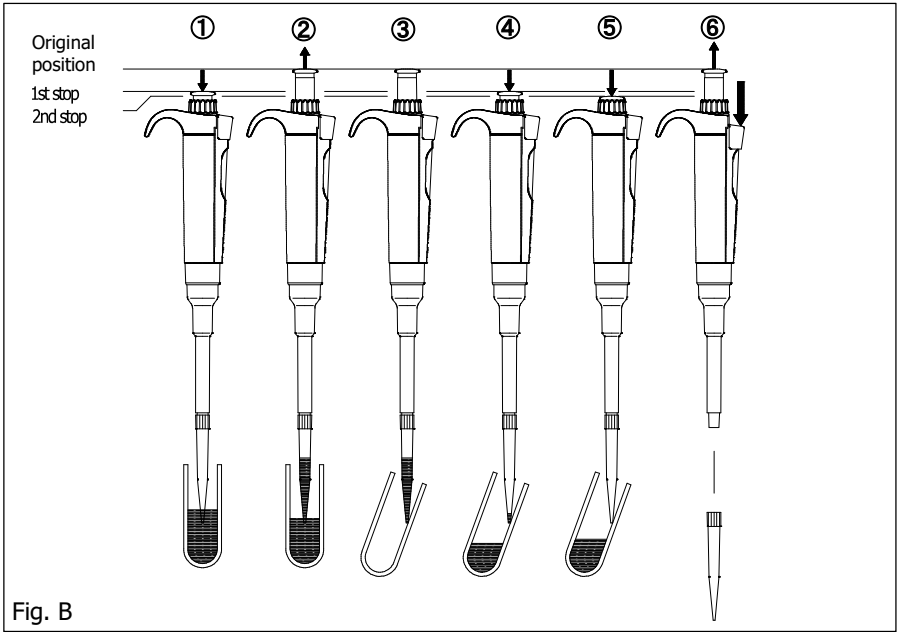


3.4 Recommendation for accurate pipetting (Technique)

1) Pre-Rinsing the tip

Higher precision can be obtained by performing the pre-rinsing of the tip. When using a fresh pipette tip for the first time and before sampling, it is important to pre-rinse the tip at least two to three times with the target solution before pipetting. Repeat the aspiration and discharge to the position of the 1st stop consecutively for two to three times (Fig. C).

When strict precision is required, this method is recommended for all kinds of liquid handling. Pre-rinsing is a fast and easy way to increase the accuracy.

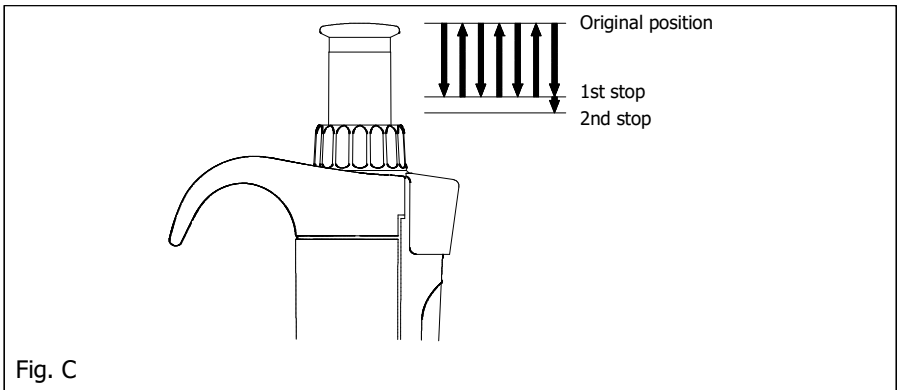

2) Handling of Viscous Solutions

After aspirating the liquid into the tip, wait for more seconds than normal viscosity before removing the tip slowly from the surface of the liquid. When dispensing, wait 2 to 3 seconds at the first stop position before pushing into the second stop position (Fig. C).

3) Small volume dispensing

Especially for volumes less than 50µL, please operate the pipette slowly and smoothly. Also, please pay close attention to the effect of evaporation loss, due to temperature and humidity.

4. Maintenance

4.1 Cleaning

When Nichipet Air's exterior is soiled, please use 70% ethanol on a clean soft cloth to wipe it off.

Also, if any symptom that is described in the "7. Troubleshooting" section occurs, disassemble and inspect the device (each part), and then check and follow the procedures in the 'Troubleshooting Table' to identify and isolate, correct and/or fix the situation or problem.



CAUTION

- ✓ Use of highly reactive liquids, may damage the device.
After using a highly reactive liquid or/and if contamination occurs, perform the disassembly and cleaning of the device, accordingly to the following method in this manual.



- ✓ In order to keep and use Nichipet AIR in its best condition, we recommend the user carries out; periodic checks and maintenance, and volume inspection/calibration of the device.
-

4.1.1 Disassembling

- 1) Turn the ejector pipe counterclockwise until it stops, and pull it out. (Fig. D)
- 2) Turn the nozzle securing nut in the direction of the arrow to remove the nozzle cylinder. (Fig. D)

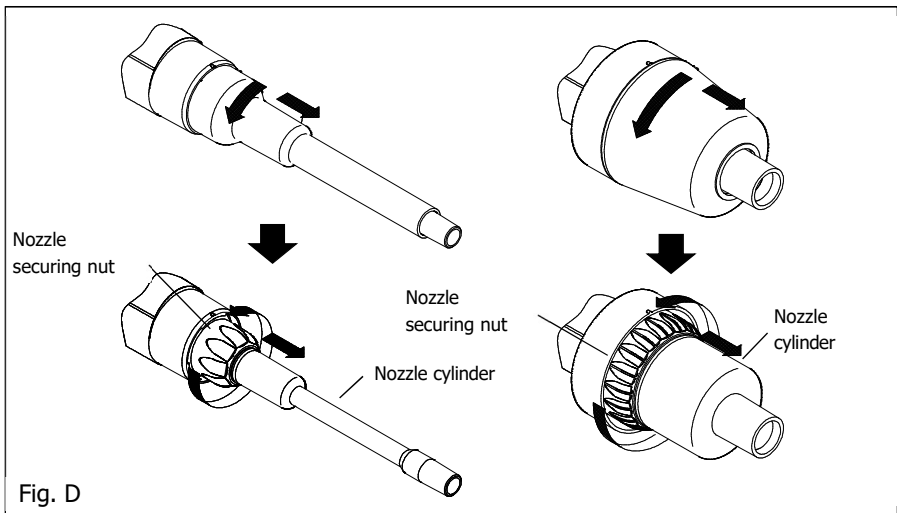



Fig. D

 CAUTION

- ✓ When removing the nozzle cylinder, disassemble it carefully, as the internal parts may pop out due to the action of the spring.

3) Take out each part as needed and accordingly.

- 2 μL , 10 μL (Fig. E, F)
The hermetic part/airtight part is integrated with the nozzle cylinder.
(It cannot be disassembled furthermore.)
- 20 μL , 100 μL , 200 μL , 1000 μL (Fig. G to J)
Take out the seal spring, O-ring retainer and O-ring.



- ✓ The shape of the O-ring retainer varies, depending on the volume type.
Please be careful and refer to the figures for details.

4.1.2 Reassembling

1) Installation of the nozzle cylinder.

- 2 μL , 10 μL (Fig. E, F)

Insert the plunger into the nozzle cylinder, and turn the nozzle securing nut clockwise, and tighten.

- 20 μL , 100 μL , 200 μL , 1000 μL (Fig. G to J)

Attach the seal spring, O-ring retainer, and O-ring to the plunger, insert the plunger into the nozzle cylinder, and turn the nozzle securing nut clockwise, and tighten.

- 5000 μL , 10000 μL (Fig. K, L)

After replacing the piston lip if necessary, insert the piston into the nozzle cylinder, and turn the nozzle securing nut clockwise, and tighten.



- ✓ When assembling, be careful not to make any mistakes in the order and the mounting orientation of the O-ring retainer and O-ring. If installed in an opposite way (upside down), airtightness cannot be maintained, causing malfunctions, such as, water leaks, accuracy errors, or liquids not being aspirated.
 - ✓ When replacing the piston lip, be careful not to damage the piston lip. Also, pay attention to the correct mounting orientation. (Right-side up.)
-

2 μ L

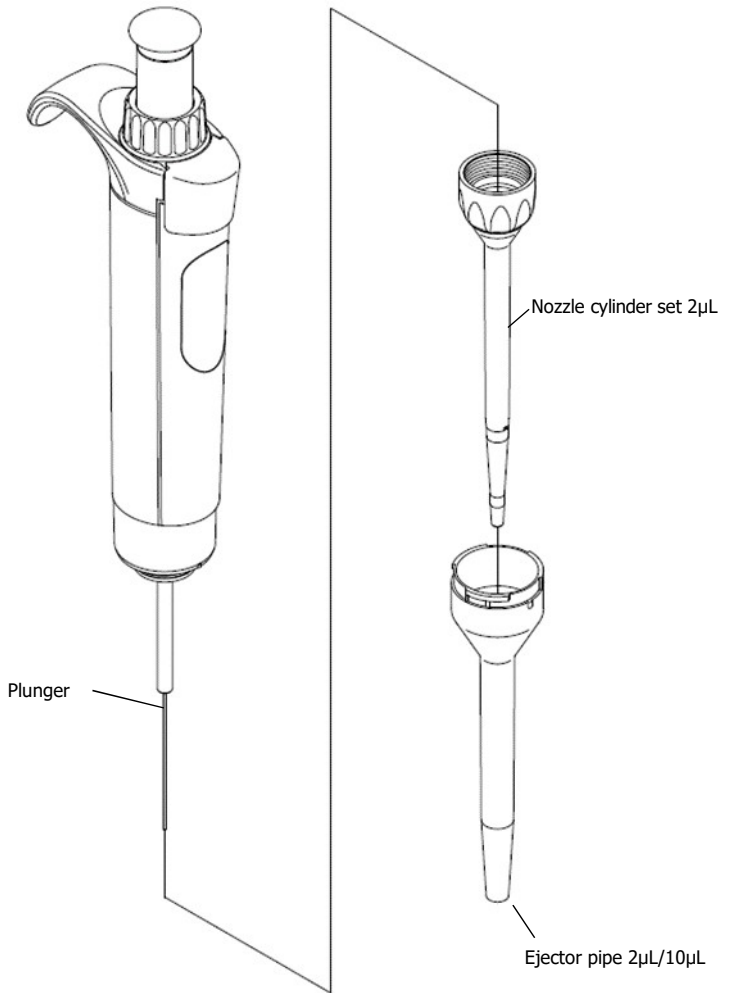


Fig. E

10 μ L

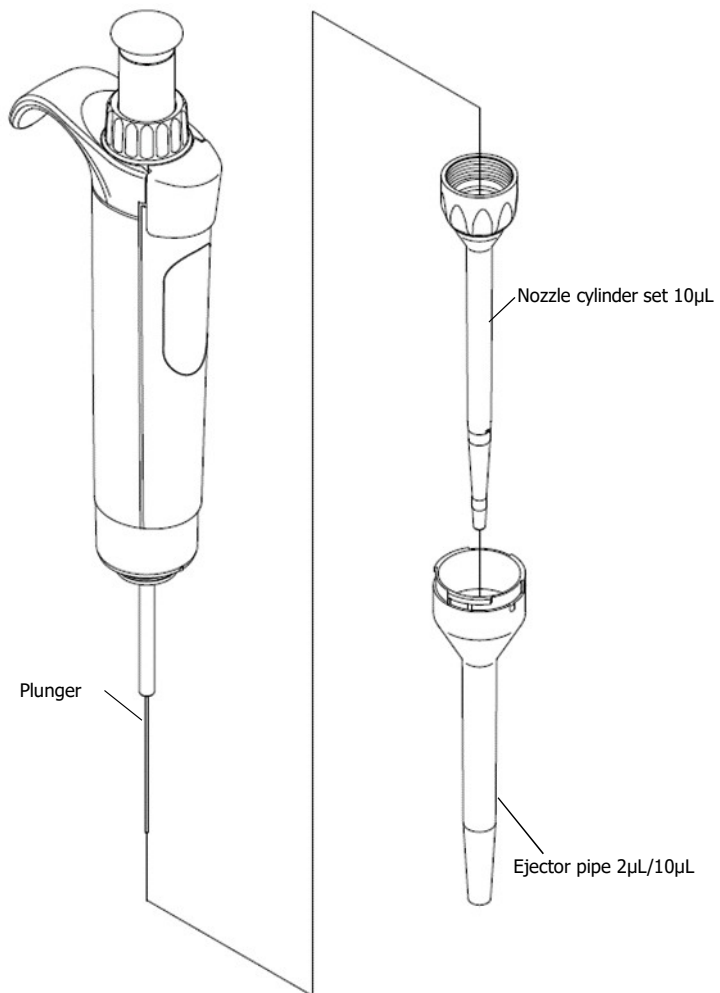


Fig. F

20 μ L

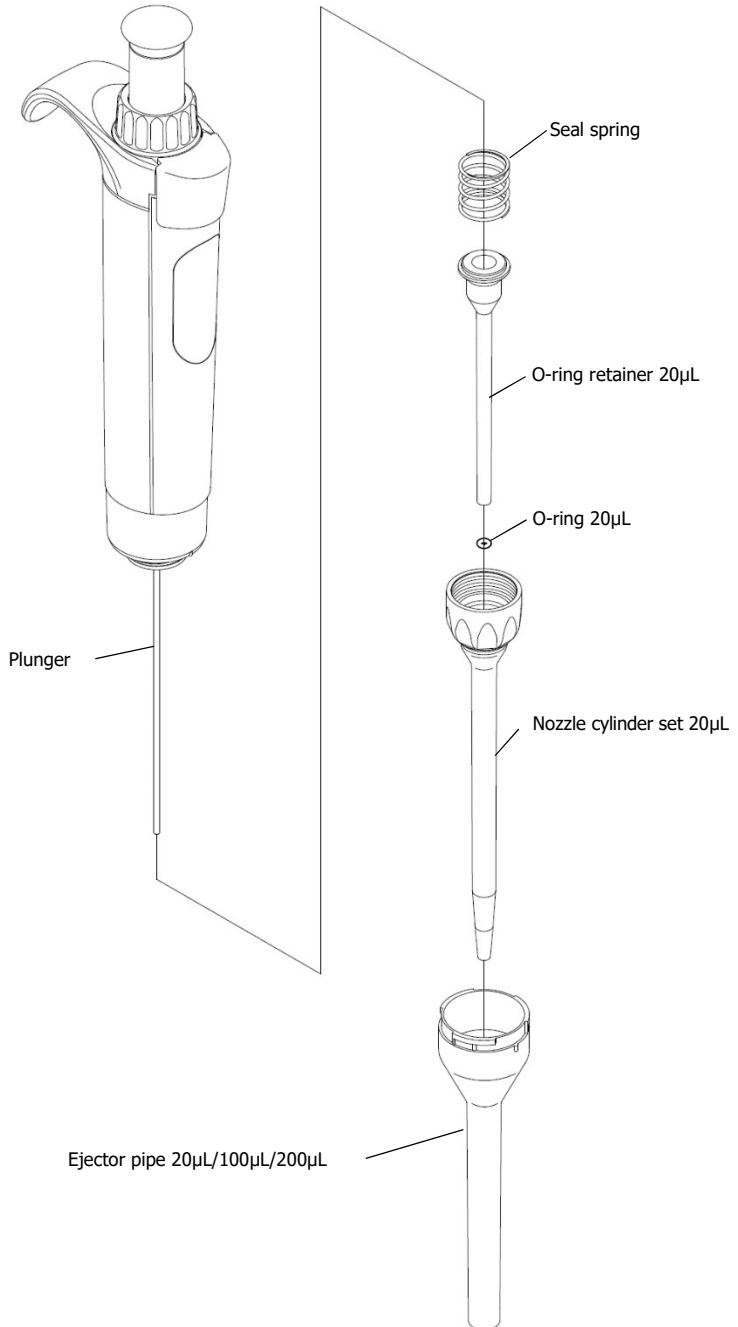


Fig. G

100 μ L

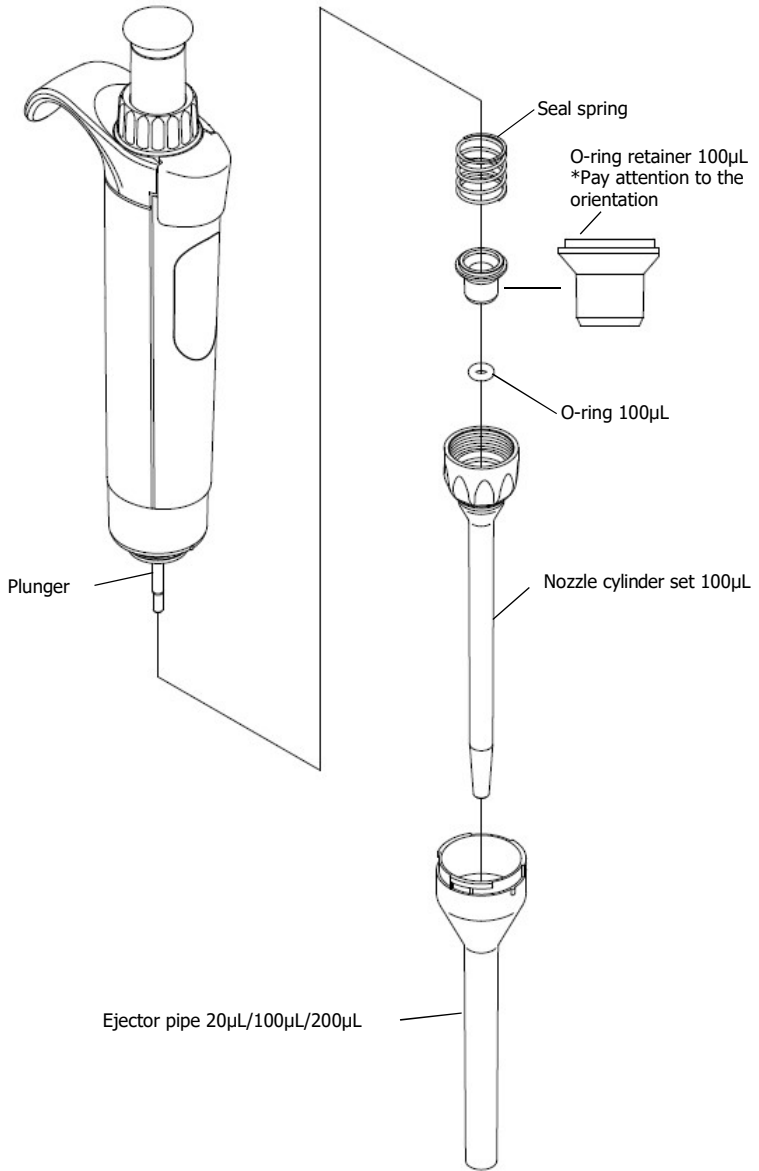


Fig. H

200 μ L

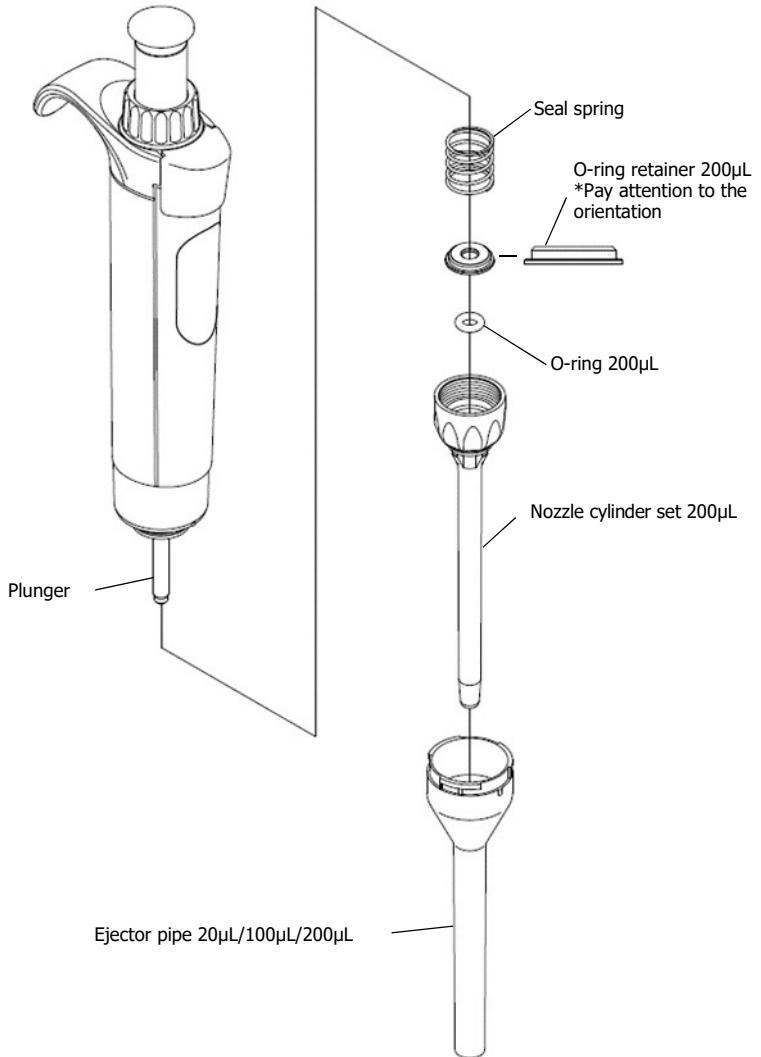


Fig. I

1000 μ L

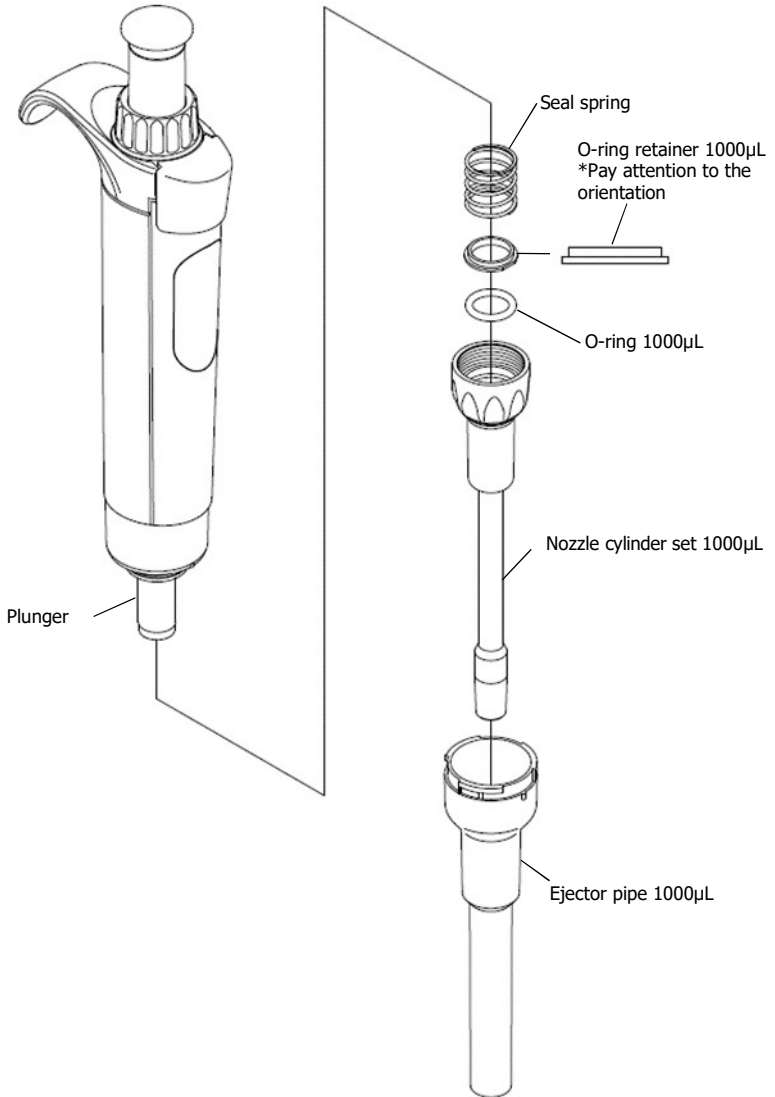


Fig. J

5000 μ L

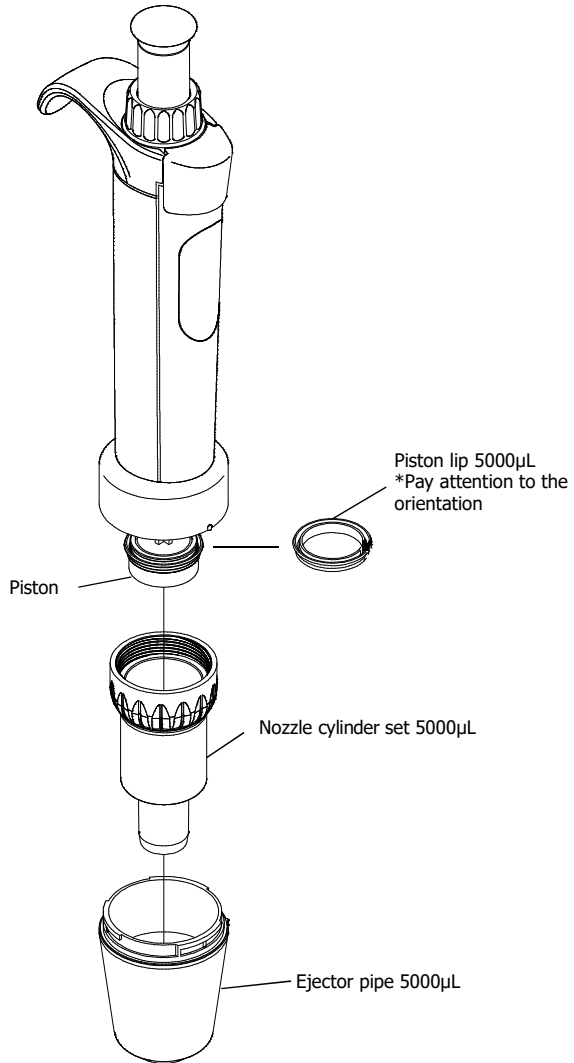


Fig. K

10000 μ L



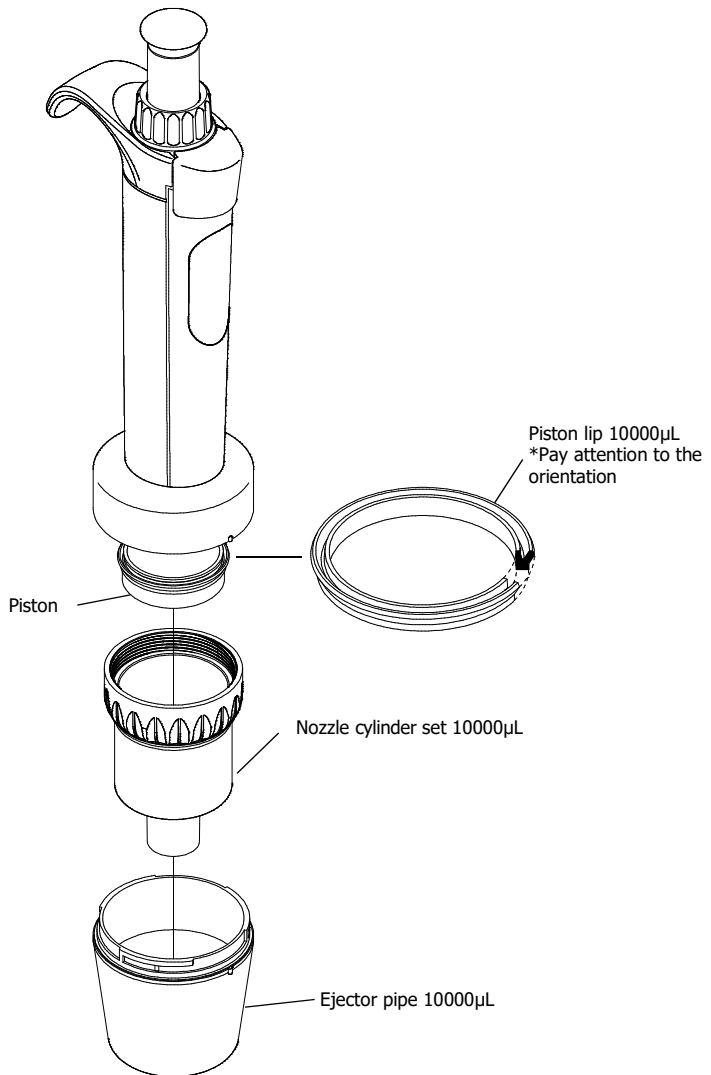


Fig. L

- 2) Attach the ejector pipe so that the alignment marks are aligned, and turn it in the direction of the arrow until it clicks. (Fig. M)
After assembling, perform the break-in operation several times to check that there is no abnormality in operation before use.
- 3) For the 5000 μL and 10000 μL types, the attached nozzle filter can be attached to the nozzle as required. Insert the nozzle filter firmly into the nozzle before use. (Fig. N)

 CAUTION

- ✓ Never directly touch nozzle filters that are contaminated with liquids that are harmful to the human body.

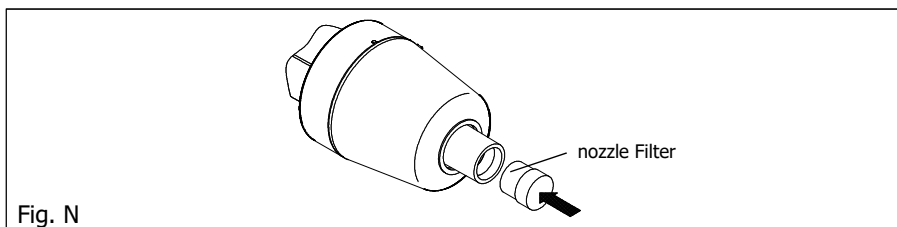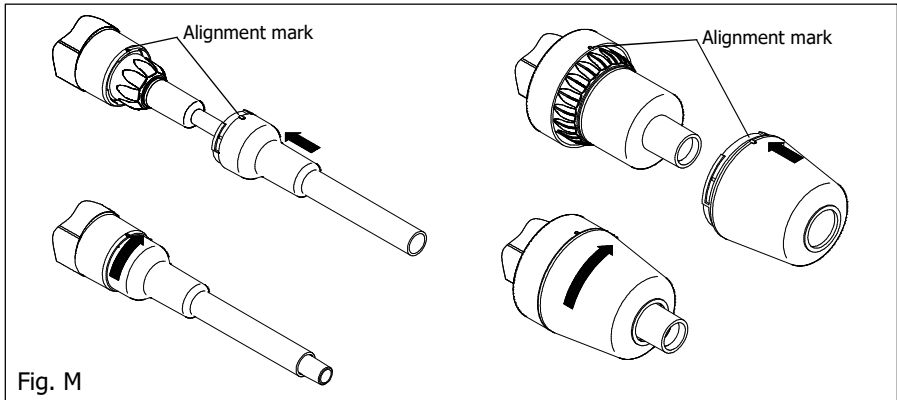

4.1.3 Lubrication/Greasing

Grease application

- 2 μL ~ 1000 μL

Depress the push button to expose the plunger, and apply a thin layer of the supplied grease to it. (Fig. O) Shaded in gray.

- 5000 μL , 10000 μL [Fig-O]

Apply the supplied grease thinly to the specified location onto the inner surface of the nozzle cylinder. (Fig. O) Shaded in gray.

 CAUTION

- ✓ Be sure to only use the specified grease. Use of any other grease will void the warranty.

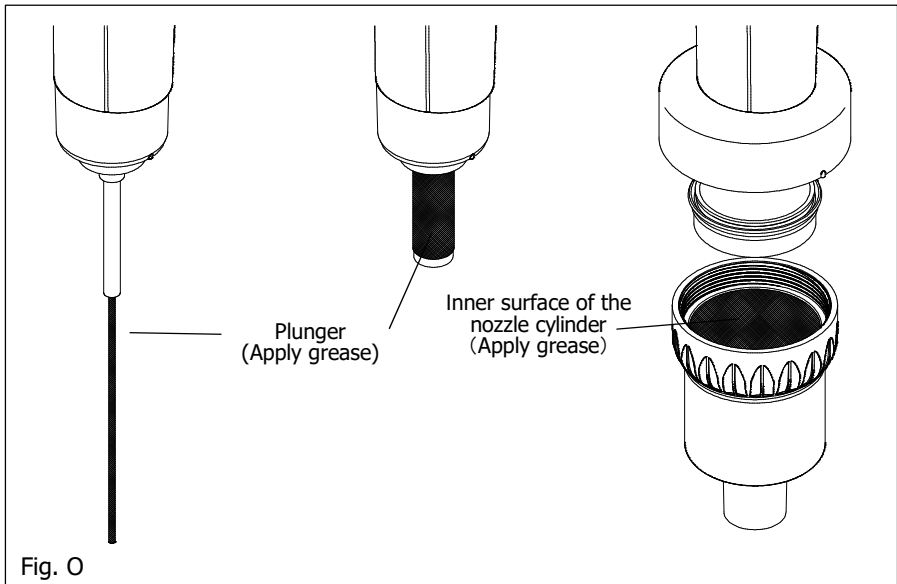


Fig. O

4.2 Autoclaving

The whole pipette is autoclavable. Carry out the autoclaving process at 121°C for 20 minutes, following the procedure below.

4.2.1 Autoclave implementation procedure

- 1) For Models: 5000µL and 10000µL, remove the nozzle filter.
- 2) When autoclaving, always check and be sure to set the volume indicator to the 'Maximum Volume' of the pipette's volume range. (This moves the plunger back/in.)
- 3) Start the autoclaving process. After autoclaving is done, please promptly dry out the pipette with the following procedure.

WARNING

- ✓ Due to high temperature and high pressure use in autoclave sterilization, it is very dangerous. Please operate equipment according to safety guidelines and standards.
-

CAUTION

- ✓ When autoclaving, do not stack items on top of each other, do not place the nozzle downward, or lean the device diagonally against anything, as this will apply load and stress to the heated structure.
Always autoclave the pipette with the nozzle facing upward and standing.
Although the pipette is made of autoclave compatible material, due to the high temperature and pressure used in the sterilizer, there is a risk that heated parts subjected to load and stress to deform.
 - ✓ Do not autoclave at temperatures above 121°C (There is a risk of causing damage.)
-

4.2.2 Drying procedure

- 1) Remove the ejector pipe according to '4.1.1 Disassembling'.
 - 2) Loosen the nozzle securing nut by making a half turn counterclockwise.
 - 3) Put the disassembled parts into a blower type constant temperature dryer to be heated. Confirm these parts are completely dried out after heating.
 - 4) After drying, confirm these parts have returned to room temperature, turn the nozzle securing nut clockwise to be fixed into the nozzle cylinder, and reattach the ejector pipe.
-

CAUTION

- ✓ Immediately after autoclaving and drying, the pipette and parts are extremely hot, so please do not touch them directly with your hands.
 - ✓ When autoclaving, there is a possibility of damage, and performance may be affected, due to other items that are in the autoclave at the same time, and/or by substances that may be present in the water that is being used in the autoclave.
 - ✓ Assembling the pipette in a heated or warm condition after drying, can lead to damage, such as stripping of the threads. Please let it cool down first. Also, if used in a heated or warm condition, accuracy will not be obtained.
-



- ✓ Accuracy and precision may change with the autoclaving conditions, and also with many other various factors. We recommend testing the accuracy and precision after autoclaving, and at other times when needed.
-

5. Specifications (Accuracy/Precision)

Table-1 Maximum Permissive Errors.

Models (Code)	volume range	Volume(μL)	Accuracy (systematic error) AC (%)	Precision (random error) CV (%)
2 μL (00-NAR-2)	0.1-2 (μL)	0.2	$\pm 12.0^*$	$\leq 6.0^*$
		1	± 2.5	≤ 1.5
		2	± 1.4	≤ 0.7
10 μL (00-NAR-10)	0.5-10 (μL)	1	± 2.5	≤ 1.8
		5	± 1.5	≤ 0.8
		10	± 1.0	≤ 0.4
20 μL (00-NAR-20)	2-20 (μL)	2	± 3.0	≤ 1.5
		10	± 1.2	≤ 0.6
		20	± 1.0	≤ 0.3
100 μL (00-NAR-100)	10-100 (μL)	10	± 3.0	≤ 1.0
		50	± 1.0	≤ 0.3
		100	± 0.8	≤ 0.2
200 μL (00-NAR-200)	20-200 (μL)	20	± 1.8	≤ 0.7
		100	± 1.0	≤ 0.3
		200	± 0.6	≤ 0.2
1000 μL (00-NAR-1000)	100-1000 (μL)	100	± 1.0	≤ 0.6
		500	± 0.8	≤ 0.2
		1000	± 0.6	≤ 0.2
5000 μL (00-NAR-5000)	500-5000 (μL)	500	± 2.0	≤ 0.6
		2500	± 0.7	≤ 0.25
		5000	± 0.5	≤ 0.15
10000 μL (00-NAR-10000)	1000-10000 (μL)	1000	± 2.0	≤ 0.6
		5000	± 0.8	≤ 0.2
		10000	± 0.5	≤ 0.15

* Accuracy and precision of 0.2 μL or less of “2 μL model” are greatly affected by the user’s sampling skills.

- Tips used: Nichiryo original tip (BMT2)
- Measurement temperature: Between 20°C to 25°C
- Relative humidity: above 50%
- Measurement medium: distilled water
- Barometric pressure, 101kPa

Volume measurement is in accordance with ISO 8655-6.

6. Calibration (Adjustments)

Perform the volume adjustment, and volume inspection, by following the procedures detailed below.

If you want to adjust the volume yourself, we recommend that you record and manage the details of the adjustment.

Please note that when the customer adjusts the volume, the accuracy and precision of the volume, and subsequent malfunctions will not be covered by the warranty.



- ✓ The volume adjustment jig used for adjustments is not included with this product. If necessary, please contact us.

6.1 Volume adjustment method

First, adjust the volume with the minimum volume for each model.

E.g. (100 μL for the 1000 μL model).

Confirm that the volume accuracy of the minimum volume is within the numerical value compared to the standard accuracy table. (Table-1)

Then proceed in order, to check the volume accuracy of the maximum volume.

<Procedure>

- 1) Measure the volume adjustment value in advance (The actual volume dispensed is the volume that is to be used for volume adjustment.) by the volume inspection method described in the next section. It is recommended to use the average value of multiple measurements in consideration of measurement deviation.

* (Example) The following describes an example in which the volume setting of the pipette is 100 μL , and the actual measured dispensing volume is "99 μL ".

- 2) Turn the push button cover in the direction of the arrow and remove it. (Fig. P)
- 3) Remove the button locking screw with a screwdriver, and remove the push button sleeve. (Fig. P)

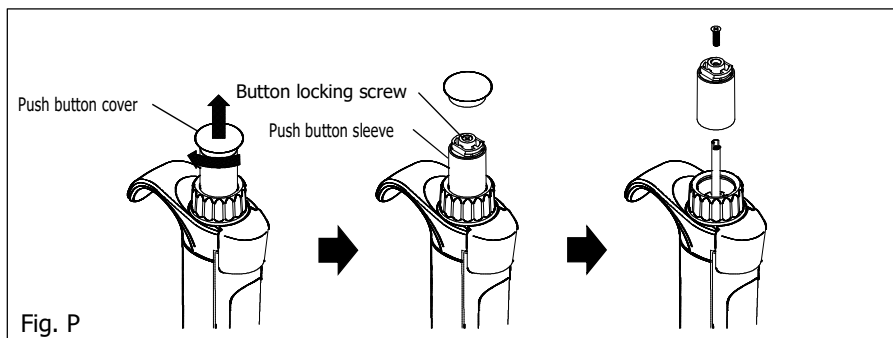


Fig. P

- 4) Set the adjustment tool projection so that it fits into the adjustment screw recess. (Fig. Q)
- 5) Hold the pipette in one hand and hold down the adjustment tool firmly so that it does not rotate. (Fig. Q)
- 6) Rotate the volume setting rotator and adjust the volume indicator value to the volume Adjustment value "99 μL ".

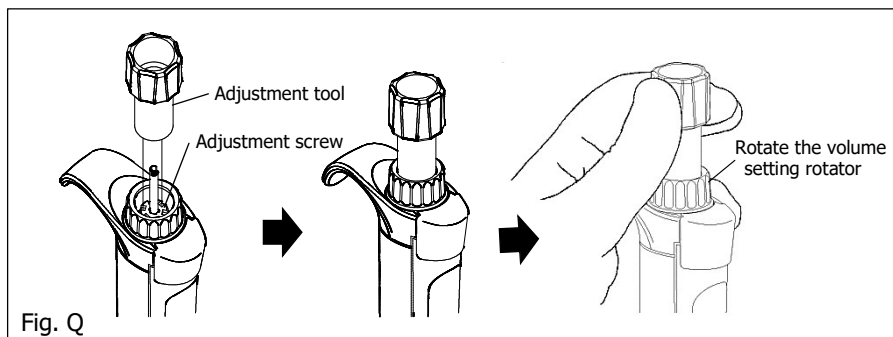


Fig. Q

- 7) Pay attention to the mating surfaces and orientation, attach the push button sleeve to the shaft in the reverse order of removal, and tighten it with the button locking screw. (Fig. R)
- 8) Align the tab on the push button cover with the D-cut on the push button sleeve, and secure it by turning it in the direction of the arrow. (Fig. R)

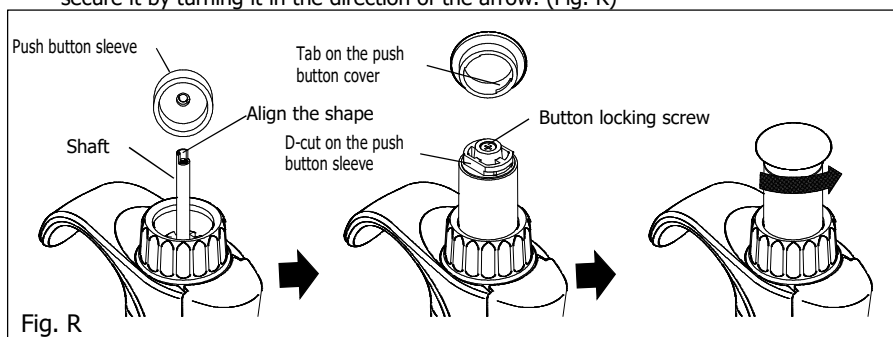


Fig. R

6.2 Volume measurement/Inspection procedure

<Procedure>

- 1) Prepare the pipette, distilled water, balance, and tip for the volume test in the room where the volume is to be measured two to three hours before the test, and make sure that there is no individual temperature difference in items.
(Temperature equilibrium)
 - * Ensure that the ambient temperature of the volume measurement environment is between 20 °C and 25 °C, and that the air from air conditioning etc. does not directly affect them.
- 2) Use the Nichiryo original tip (volume compatible one) and always attach it to the pipette from the rack.
- 3) Use distilled water as a measurement sample, pipette the sample into the container on the balance, and measure it by gravimetric method.
 - * When measuring, be sure to use a container with a lid on it for the container on the balance. Also, put a small amount of distilled water in advance in the container.
(Evaporation factor.)
- 4) Read the mass (mg) measured on the balance, and convert the value (correction factor for distilled water) to obtain the dispensed measurement volume (μL).

$$\text{Measurement volume } (\mu\text{L}) = \text{Measurement mass (mg)} \times \text{Correction factor for distilled water (Table-2)}$$

5) Calculate the measured value, and compare with the standard accuracy (Table-1) to confirm the accuracy and 11ibility. Perform the volume measurement at least 5 times.

<Reference> Use the following formula to calculate the value of the accuracy and reproducibility.

$$[\text{Precision (Accuracy)}] (\%) = (\text{Average Volume Value} - \text{Set Volume}) / \text{Set Volume} \times 100$$

$$[\text{Reproducibility}] (\%) = \text{Standard Deviation} / \text{Average Volume Value} \times 100$$

[Standard Deviation]


$$S_r = \sqrt{\frac{\sum_{i=1}^n (V_i - \bar{V})^2}{n-1}}$$

Table-3 Z correction factor for distilled water (Mass / Volume Conversion Factor)

Temperature (°C)	Air Pressure (kPa)			
	95.0	100.0	101.3	105.0
20.0	1.0028	1.0028	1.0029	1.0029
20.5	1.0029	1.0029	1.0030	1.0030
21.0	1.0030	1.0031	1.0031	1.0031
21.5	1.0031	1.0032	1.0032	1.0032
22.0	1.0032	1.0033	1.0033	1.0033
22.5	1.0033	1.0034	1.0034	1.0034
23.0	1.0034	1.0035	1.0035	1.0036
23.5	1.0036	1.0036	1.0036	1.0037
24.0	1.0037	1.0037	1.0038	1.0038
24.5	1.0038	1.0039	1.0039	1.0039
25.0	1.0039	1.0040	1.0040	1.0040

7. Troubleshooting

Symptom	Possible cause	Remedy
Tip cannot be ejected.	The nozzle securing nut is loose	Securely, tighten up the nozzle cylinder.
	The ejector pipe is loose	Replace the ejector pipe correctly.
Pipette fails to aspirate liquid.	Nozzle tip is clogged (Foreign matter adhered)	Clean or replace nozzle cylinder parts
	The nozzle securing nut is loose	Securely, tighten up the nozzle cylinder.
	O-ring and O-ring retainer are assembled in reverse order	Replace the O-ring and O-ring retainer by following the instruction on this manual.
	Grease in the hermetic part/ airtight part is depleted	Apply grease by following the instruction on this manual.
Extracted liquid leaks from the tip.	The nozzle securing nut is loose	Securely, tighten up the nozzle securing nut.
	The nozzle is loose	Replace the nozzle cylinder set
	The O-ring is loose	Replace the O-ring. *Replace the nozzle cylinder set for 2 μ L and 10 μ L.
	The piston lip is loose	Replace the piston lip.
	The tip is loosely attached.	Reattach the same loosened tip, or with a new one firmly.
	Grease in the hermetic part/ airtight part is depleted	Apply grease by following the instruction on this manual.
Push button moves stiffly.	The liquid has aspirated and leaked inside the nozzle cylinder.	If the push button does not work well after dispensing, or it is sticking to the body, disassemble the pipette and wash/clean every part (or wipe down every part with a soft cloth). If some parts get rusty or corroded inside the body, replace the part(s) with new one(s).
	Grease in the hermetic part/ airtight part is depleted	Apply grease by following the instruction on this manual.

-
-  ✓ When the pipette cannot be fixed after examining and conducting the above mentioned procedure, immediately stop using the pipette and ask us or our agent to repair it.
Before bring the pipette for repair, be sure to check whether it has been contaminated with microbes, and/or harmful or toxic substance. Otherwise, it cannot be undertaken the repair.
-

8. Replacement parts list

8.1 Consumables

•Tip (Autoclavable)

Code	Applicable models	Length of tip (External size)	Q'ty
00-BMT2-UT	2μL、10μL	31.5mm	1000
00-BMT2-SG	20μL、100μL、200μL	53.0mm	1000
00-BMT2-LG	1000μL	81.9mm	1000
00-BMT2-X	5000μL	132.0mm	200
00-BMT2-ZS	10000μL	171.2mm	200

•Racked tip (Autoclavable)

Code	Applicable models	Q'ty
00-BMT2-UTWR	2μL、10μL	960 (96pcs x 10 cases)
00-BMT2-SGR	20μL、100μL、200μL	960 (96pcs x 10 cases)
00-BMT2-LGR	1000μL	960 (96pcs x 10 cases)
00-BMT2-XR	5000μL	100 (50pcs x 2 cases)
00-BMT2-ZSR	10000μL	80 (40pcs x 2 cases)

8.2 Spare parts list

Code	Replaced parts name	Remarks	Volume
00-NAR-G1000	Seal spring	-----	20uL/100μL/200μL 1000uL
00-NAR-ABC2	Nozzle cylinder set 2μL	O-ring and O-ring retainer included	2μL
00-NAR-ABC10	Nozzle cylinder set 10μL	O-ring and O-ring retainer included	10μL
00-NAR-A20	Nozzle cylinder set 20μL	-----	20μL
00-NAR-A100	Nozzle cylinder set 100μL	-----	100μL
00-NAR-A200	Nozzle cylinder set 200μL	-----	200μL
00-NAR-A1000	Nozzle cylinder set 1000μL	-----	1000μL
00-NAR-A5000	Nozzle cylinder set 5000μL	-----	5000μL
00-NAR-A10000	Nozzle cylinder set 10000μL	-----	10000μL

Code	Replaced parts name	Remarks	Volume
00-NAR-E10	Ejector pipe 2μL/10μL	-----	2μL/10μL
00-NAR-E200	Ejector pipe 20μL/100μL/200μL	-----	20μL/100μL/200μL
00-NAR-E1000	Ejector pipe 1000μL	-----	1000μL
00-NAR-E5000	Ejector pipe 5000μL	-----	5000μL
00-NAR-E10000	Ejector pipe 10000μL	-----	10000μL
00-NAR-C20	O-ring retainer 20μL	-----	20μL
00-NAR-C100	O-ring retainer 100μL	-----	100μL
00-NAR-C200	O-ring retainer 200μL	-----	200μL
00-NAR-C1000	O-ring retainer 1000μL	-----	1000μL
00-NAR-B20	O-ring 20μL	-----	20μL
00-NAR-B100	O-ring 100μL	-----	100μL
00-NAR-B200	O-ring 200μL	-----	200μL
00-NAR-B1000	O-ring 1000μL	-----	1000μL
00-NAR-B5000	Piston lip 5000μL	-----	5000μL
00-NAR-B10000	Piston lip 10000μL	-----	10000μL
00-NAR-F15000	Nozzle filter (10pcs)	-----	5000μL /10000μL
00-NAR-GRS	Grease	-----	All
00-NAR-AT	Volume adjustment tool	-----	All


Please note that the specifications of the accessories may be changed without notice.
Always check our website for the latest specifications and information.

* Copying/Reprinting the manual in whole or in part without permission, is prohibited by law.

Inspection and Calibration Statement

The enclosed pipette was tested and calibrated under closely controlled environmental conditions to ensure that it meets published calibration specifications. The precision and accuracy results obtained for this pipette are provided on the enclosed calibration certificate. Because temperature and humidity conditions affect the calibration results of liquid measurement devices, your pipette should be calibrated under conditions of use. The calibration results obtained in your laboratory may vary from our results, due to differences in the environmental testing conditions.

Information on repair or servicing, when contacting your local distributor.



Authorized Representative:



Emergo Europe B.V.
Prinsessegracht 20
2514 AP, The Hague The Netherlands

Manufacturer :

NICHIRYO CO.,LTD.



Head office & Factory

2760-1 Nishikata, koshigaya-Shi, Saitama 343-0822, Japan
TEL: +81-48-989-1301 FAX: +81-3-6273-7944

Tokyo Main office (Sales Division)

Sakura building 3F, 1-10-1 Kandanishiki-cho, Chiyoda-ku, Tokyo 101-0054,
Japan

TEL: +81-3-6273-7652 FAX: +81-3-6273-7944

URL: <http://www.nichiryo.co.jp/>

E-mail: i-sales@nichiryo.co.jp