
ENGLISH

*Other languages available on
our website: www.gilson.com.*



PIPETMAN *Concept*[®]

1	INTRODUCTION	3	10	SYSTEM MENU	(CONTINUED)
2	PARTS CHECK LIST AND ACCESSORIES	3		Calibration	20
	Accessories	3		Standard Readjustment	20
3	GETTING STARTED	4		Quick Adjustment	21
	Battery charging	4		Factory Settings	21
	Setting-up	4		Maintenance	21
	Initializing	5		Disassembly	21
	Standby Screen	5		Service Info	22
4	DESCRIPTION	5		Service Settings	22
	Pipette	5		Maintenance Alarm	22
	Keypad	6		Pipette Info	22
	Screen (LCD)	6		Personalization	22
	Tip-ejector Extension	7	11	USER MAINTENANCE	23
5	OPERATION	7		Maintenance Warnings	23
	Switching On	7		Maintenance Operations	23
	Thumbwheel	7		Maintenance Operations for Single channel	24
	Start Button	8		Tip-holder and Tip-ejector	24
	Speed Buttons	8		Changing the Tip-ejector	24
	Direction Button	8		Changing the Tip-holder	24
	Mode Buttons	8		Changing the O-ring (or seal for C10)	24
	Reset Button and Connectors	8		Servicing the Piston	25
	Tip-Ejector Button	8		Removing the Piston	25
6	PIPETTING MODES	9		Maintenance Operations for Multichannel	26
	Overview	9		Removing and reassembling the Head	26
	Selecting	9		Removing the Plastic Cover...	26
	Aborting the Active Mode	9		Servicing the Ejector-cover...	27
	Mode Description	10		Reassembling the Piston Assemblies...	27
	AUTO	10		How to Lubricate the Piston (except for C10)	28
	AUTO + MIX	11	12	CLEANING AND DECONTAMINATION	28
	MANUAL	12		Cleaning	29
	REPETITIVE	13		External	29
	REVERSE	14		Internal	29
	Programming Modes	15		Decontamination	29
	DILUTE	15		Autoclaving	29
	DILUTE AND MIX	15		Chemical Decontamination	30
	MULTIPLE ASPIRATES	15	13	LEAK TEST	30
	DISTRIBUTION WITH TIMER	15		C10 to C300 Single and Multichannel	30
7	GILSON DIAMOND[®] TIPS	15		C1200 to C10ml	31
8	PIPETTING TECHNIQUES	16	14	TROUBLESHOOTING	31
	Guidelines for Good Pipetting	16	15	ACCESSORIES & REPLACEMENT PARTS	32
	Aspirate and Dispense	17		Accessories	32
9	GLP FEATURES	18		Replacement Parts for Concept Single channel	32
	General	18		Replacement Parts for Concept Multichannel	34
	Cycle counters	18	16	SAFETY PRECAUTIONS...	34
	Alarms	18	17	SPECIFICATIONS	36
10	SYSTEM MENU	19	18	GILSON MAX. PERMISSIBLE ERRORS	37
	Configuration	19		EC DECLARATION OF CONFORMITY	38
	Beeper	19		NOTES	39
	Screen contrast	19			
	Volume limit	19			

1 INTRODUCTION

Thank you for choosing Gilson Pipetman® Concept - the latest and most user-friendly of motorized pipettes. It is another quality product from Gilson, which is fully ISO8655 compliant, CE labeled (conforms to the EC directives on *in vitro* diagnostic medical devices, electromagnetic compatibility and safety).

To ensure the best performance from your Gilson pipette you should always use Gilson Diamond® Tips (in accordance with ISO8655) to complete your pipetting system, because Diamond Tips were used to establish the specifications cited in Chapter 17.

Please refer to Chapter 16 for Safety precautions and limitations of use.

2 PARTS CHECK LIST AND ACCESSORIES

The following items are supplied in the box:

- Pipetman Concept pipette
- Battery block
- Sample Diamond Tips (Tipack rack or for C5000 and C10ml a bag of tips)
- Guarantee and quality certificate
- User's Guide & Quick Guide
- Safety bag
- Tip-holder reassembly tool (Multichannel models only)
- Tube of lubricant
- Identification tags
- Tip-ejector extension (C10 model only)

Accessories

The following item may be supplied either in the box or separately by your Gilson distributor:

- AC adaptor (four region types are available: Europe, UK, USA/Japan, Australia).



The following items are **not** supplied in the box:

- Rapid charging and storage stand (AC adaptor not included)
- PC Connection kit (includes PC cable plus programming and maintenance software)
- Additional battery block

 Please contact your Gilson Distributor for these accessories. Order with the reference numbers given in Chapter 15.

3 GETTING STARTED

- 1) Slide the battery block into the pipette (see fig. 1).
- 2) Your Gilson distributor supplies an AC adaptor that is suitable for your country – either in the pipette box or separately. **You must only use an original Gilson AC adaptor specific to this product.**
- 3) Connect the AC adaptor to a suitable AC power supply and plug the adaptor into the pipette (see figure 2). If you have a charging stand, then you must first place the pipette on the stand and plug the adaptor into the stand. It takes two to three hours to fully charge the battery or one hour for 80% charge. We strongly recommend you fully charge the battery before using the pipette.

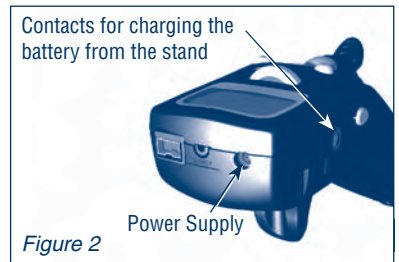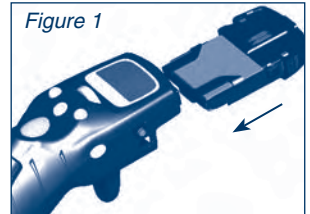


Battery Charging

When charging the pipette you see the following screen:



Get a second battery block – that way one can be charged while the pipette is in use (you can plug the battery block into the charging stand).



Version number of the firmware

Setting-up

- 1) Set the position of the adjustable hook to the position of maximum comfort for you size of hand (see figure 3). Loosen the retaining screw (do not undo completely), slide the hook into the most comfortable position, and then retighten the screw.
- 2) Fit Gilson Diamond Tips appropriate for the model of Pipetman Concept that you are using (see Chapter 7).




You must always fit a tip before using any pipette.


- 3) Rotate the tip-adjustment force regulator until you reach the optimum force for you and the type of tip being used (see figure 3).
- 4) Optionally, you may personalize the name of your pipette (see Chapter 10).

Initializing

Press any button to activate the pipette. You then see the start-up screen:

Select your mode (see Chapter 6) and enjoy using your Pipetman Concept.


 *To get used to the pipette, we recommend you select the AUTO mode.*



Standby Screen

Pipetman Concept goes to stand-by after 3 minutes of inactivity. Press any button to reactivate the pipette. If you do not press one of the buttons within 3 minutes of the end of the current cycle, you will see the standby screen:

When you next press a button, the software reinitializes the piston.



4 DESCRIPTION

Pipette (figure 3)

- ① Adjustable tip-ejector button, can be positioned for left or right-handed operation.
- ② Ergonomic, adjustable hook, to make the pipette more comfortable to use, and to reduce fatigue.
- ③ Identity-tag window (see GLP features).
- ④ Connecting nut – links handle to the lower part.
- ⑤ Tip-ejector stroke adjustment-wheel – Force Regulator.
- ⑥ Tip-ejector: removable to access piston assembly and tip-holder.
- ⑦ Optimized tip-holders to reduce tip fitting and ejection forces – removable for cleaning and servicing.

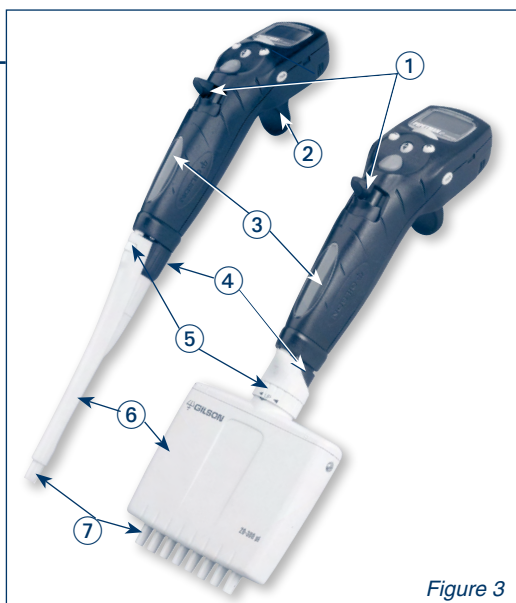


Figure 3

Keypad (figure 4)

The following buttons are used to control the pipette.

- ① Thumbwheel to set the volume and other system parameters: setting by rolling, and validating by clicking,
- ② Reset button, to initialize the pipette (see chapter 5),
- ③ Contacts for charging the battery from the stand (see chapter 15),
- ④ Two buttons (+) and (-) to adjust the speed,
- ⑤ Two mode buttons, one for right handed and one for left handed, to select the requested mode,
- ⑥ A button to inverse direction of piston motion (Manual mode),
- ⑦ Start button, to aspirate and dispense,
- ⑧ A button for tip ejection.


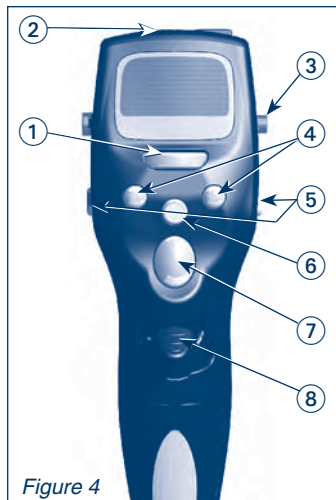


Figure 4

Screen (LCD)

Typically, the LCD screen is used to display:

- The available modes and the parameters required for a specific mode.
- Information relating to the current manipulation in real time.
- Battery state (4 levels)
- Piston direction and motion in real time (see Chapter 6).
- Configuration and maintenance information (see Chapter 10).
- Cycle counter (see Chapter 9).
- Warning messages, which appear in the place of volume (refer to Chapter 14 for the full list).

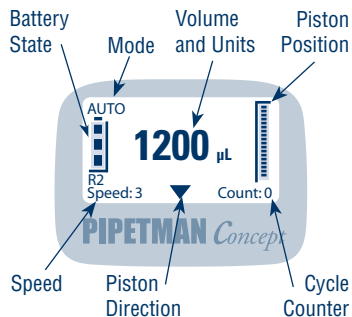


Tip-ejector Extension (only with C10 model)

In order to eject D10 tips, tip-ejector extensions are supplied with C10 pipettes (figure 5).

The tip ejector extension, which is made of PVDF (polyvinylidene difluoride), is autoclavable.

Do the following to fit a tip extension.

- 1) Hold the pipette with the LCD uppermost and hold the extension with the slot uppermost,
- 2) Slide the extension over the tip-holder,
- 3) Push the extension firmly onto the end of the tip-ejector until it clicks into place (see opposite).
- 4) To remove a tip-ejector extension (see opposite):
 - a) Hold the pipette in one hand and grip the extension with the other.
 - b) Gently twist the extension (either direction) and pull it away from the pipette.

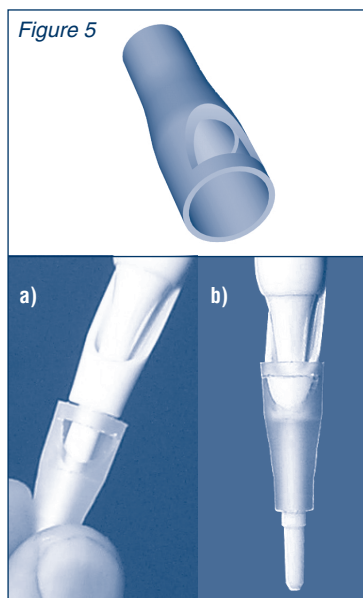

5 OPERATION


Switching On (figure 6)

Press any button to activate the pipette. After pressing a button, if nothing shows on the screen, check that the battery is charged (see Chapter 3).

Thumbwheel


There are two ways of using the thumbwheel: by rotating in either direction or by pressing inward sharply (clicking). For example, to set the volume:

- 1) Click the thumbwheel to unlock the volume.
- 2) Rotate the thumbwheel to set the volume.
- 3) Click the thumbwheel to lock the volume.

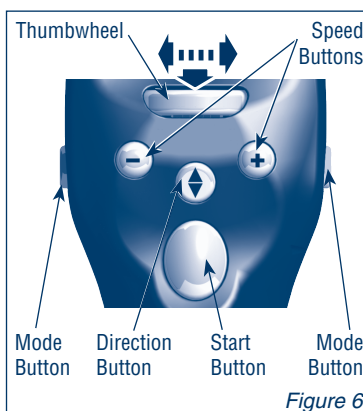

PIPETMAN *Concept*[®]

The thumbwheel is also used to select parameters and to choose from the System menu. However, it always operates in the same manner; click then turn to select and click again to confirm your choice. These options are explained in the following text at the appropriate point.

 *When setting the volume, use a sharp motion on the thumbwheel to move rapidly through the volume range or use a slow and deliberate motion to fine tune the volume.*

Start Button



This button is the equivalent of the plunger on a manual pipette. However, very little force is needed to operate it. A simple click is all that is needed to aspirate and dispense or to purge the pipette.

Speed Buttons



These buttons are used to change the speed (which may be set from 1 to 5) of a pipetting cycle: + to increase the speed – to decrease the speed.

 *The speed can be changed before or during a pipetting cycle.*

Direction Button



Press this button to change the direction in which the piston is moving. The arrow on the screen will change accordingly.

 *This button is only active in the MANUAL mode (see Chapter 6).*

Mode Buttons




There are two buttons located at either side of the pipette: one each for left- or right-handed operators.

Press either of these buttons to display the mode menu on the screen (see Chapter 6). Pressing both at the same time will switch the pipette to System menu (see Chapter 10).

Reset Button and Connectors (figure 7)

The reset button is recessed at the back of the pipette between the power supply and the PC connector. Insert a small plastic probe or a tip and press to reinitialize the pipette.

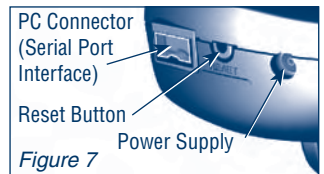

Tip-Ejector Button (figure 8)

This is a mechanical button that can be set for left- or right-handed users.



6 PIPETTING MODES

Overview


Pipetman Concept has five pre-programmed modes. The “AUTO” mode is the recommended for the new user to become familiar with the operation of Pipetman Concept.

Selecting

Press either of the “Mode” buttons. The “Mode” menu shows on the LCD screen. The active mode is indicated.

To select another mode, scroll the different modes by turning the thumbwheel, then press the thumbwheel to confirm.

In each of the modes listed below the parameters last used are kept in memory until you change them.

 After a few seconds the display returns to the last mode used, if no new mode is selected.


The REVERSE mode can be replaced by another programmed mode that can be uploaded by the user with a PC Connection Kit (optional). The kit, which includes a PC cable, programming and configuration software, can be obtained from your usual Gilson representative (the reference number is F30755).

Reminder: Pressing both mode buttons at the same time switches the pipette to System menu (see Chapter 10).

Aborting the Active Mode

If you press one of the mode buttons **during the current cycle** the following is displayed:

If you do not press the **START** button within a few seconds you are sent back to the previous screen.



Mode Description

AUTO

a) Description:


This is the simplest mode. Aspirate and dispense are initiated using the **START** button.



b) Protocol:

- i) Click on the thumbwheel to unlock the volume setting – the current volume will flash.
- ii) Set the sample volume: turn the thumbwheel until you see the selected volume displayed on the screen, then press the thumbwheel to lock the volume – you cannot dispense until this is done.
- iii) Set the speed (optional): press the +/- keys to increase or reduce the speed (default is 5). The speed can be changed before or during a pipetting cycle.

c) Functionality:

- i) Immerse the tip in the liquid to be aspirated.
- ii) To aspirate: click (press and release) the **START** button and wait until the motor stops (check piston position indicator).
- iii) To dispense: click (press and release) the **START** button. Three things happen: sample dispense, automatic purge and piston reset to zero. However, if you keep the button pressed until the end of the dispense cycle (when the motor stops) the piston reset takes place **after** you release the **START** button again. This feature enables you to remove the tip from the liquid – otherwise liquid would be re-aspirated when the piston resets.


 In this mode the user has access to a cycle counter, which is incremented after each pipetting cycle. It counts up to 999 before starting again at zero. The counter is reset to zero each time the volume is changed or by pressing twice on the thumbwheel.

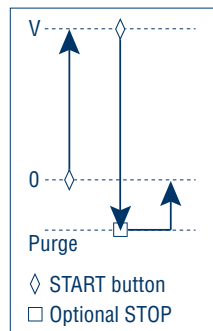

AUTO + MIX

a) Description:

This mode operates in the same way as AUTO, but is followed by a mixing phase, which is achieved by repeatedly aspirating and dispensing.





b) Protocol:

- i) Set the sample volume: with “AUTO” flashing on the screen, click the thumbwheel then turn it until you see the selected volume displayed, then press the thumbwheel to lock the volume.
- ii) Set the mix volume: with “MIX” flashing on the screen, turn the thumbwheel until you see the selected volume displayed, then press the thumbwheel to lock the volume. Then “AUTO” is displayed again. The default is the sample volume previously selected, to accept this value for mixing simply press the thumbwheel for the second time.
- iii) Set the speed (optional): press the +/- keys to increase or reduce the speed (default is 5). The speed can be changed before or during a pipetting cycle.

c) Functionality:

- i) Immerse the tip in the liquid to be aspirated.
- ii) To aspirate: click (press and release) the **START** button and wait until the motor stops (check piston position indicator).
- iii) To dispense: click (press and release) the **START** button. Three things happen: sample dispense, automatic purge and piston reset to zero. However, if you keep the button pressed until the end of the dispense cycle (when the motor stops) the piston reset takes place **after** you release the **START** button again.
- iv) To mix: press the **START** button again; mixing continues for as long as you keep the **START** button pressed. Release the **START** button to complete the current mixing cycle.
- v) Purge: click on **START** to purge and reset the piston. “BLOW OUT” appears on the screen until the piston has reset to zero.

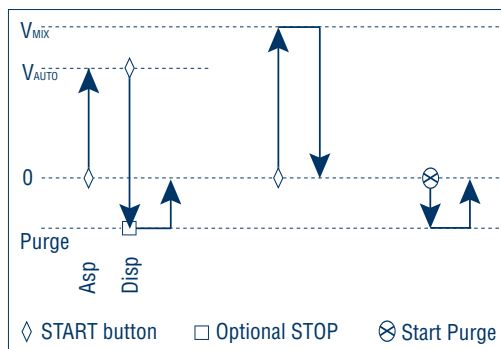

 During the normal aspirate and dispense phase the word “AUTO” appears; the volume displayed is the sample volume. During the mixing phase the word “MIX” appears; the volume displayed is the mix volume.

In this mode the user has access to a cycle counter, which is incremented after each pipetting cycle. It counts up to 999 before starting again at zero. The counter is reset to zero each time the volume is changed.

MANUAL

a) Description:

This mode simulates the way in which a manual pipette is operated. The user can stop and start the aspirate and dispense phases at will.


This enables you to load a gel or measure a sample volume. You can also set a volume limit before aspirating a liquid phase.




b) Protocol:

- i) Set the volume limit (optional): click on the thumbwheel than turn it until you see the selected volume limit (V_{max}) displayed on the screen, then press the thumbwheel to lock the volume – you cannot dispense until this is done. If you do not set a volume, the default volume is the nominal volume of the pipette.
- ii) Set the speed (optional): press the +/- keys to increase or reduce the speed (default is 5). The speed can be changed before or during a pipetting cycle.

c) Functionality:

- i) To aspirate: keep the **START** button pressed. You can stop by releasing the **START** button and restart by pressing it again. You can aspirate until V_{max} or the nominal volume is reached.
- ii) Press the **DIRECTION** button to change the direction in which the piston moves from up to down (see direction arrow on the display). You can change direction at any time during an aspirate or a dispense cycle.
- iii) Dispense: keep the **START** button pressed. At any time, you can stop by releasing the **START** button and restart by pressing it again. When the volume reaches 0.0 μL , dispensing stops.
- iv) Purge: click on **START** to purge and reset the piston. "BLOW OUT" appears on the screen until the piston has reset to zero.

 The volume of liquid present in the tip is permanently displayed in real time. As a consequence, you can use the MANUAL mode to measure unknown volumes. However, take care to reset the selected volume (V_{max}) to the nominal volume (e.g. 1200 μL for a C1200).

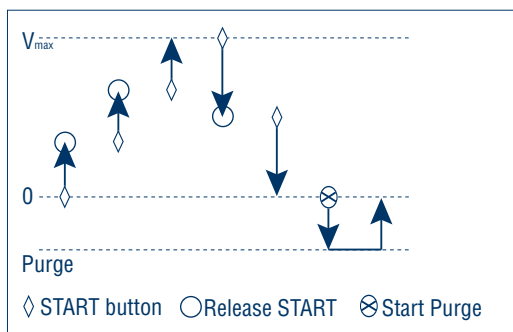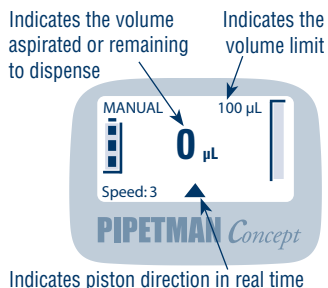

REPETITIVE

a) Description:

This mode distributes a number (N) of equal aliquots. You supply the aliquot volume (AV) and the pipette automatically calculates the number from the nominal volume (NV) of the pipette as follows: $N = NV/AV$ (e.g. 120 $\mu\text{L} \times 10$ for C1200).

b) Protocol:

- i) Set the aliquot volume: click the thumbwheel, the default volume flashes. To change the volume turn the thumbwheel until you see the required volume displayed on the screen.
- ii) Then press the thumbwheel to lock the volume and calculate the number of aliquots.

The number of aliquots flashes. You can change the number of aliquots using the thumbwheel or simply press the thumbwheel to accept the number displayed.



- iii) Set the speed (optional): press the +/- keys to increase or reduce the speed (default is 5). The speed can be changed before or during a pipetting cycle.


c) Functionality:

- i) Immerse the tip in the liquid to be aspirated.
- ii) To aspirate*: click (press and release) the **START** button and wait until the motor stops (check piston position indicator).
- iii) To dispense: click (press and release) the **START** button "N" times to sequentially dispense the aliquots. The number of aliquots left to dispense is displayed on the screen.

- iv) iv) "BLOW OUT" appears on the screen when no aliquots are left to dispense. Click on **START** to purge and reset the piston. However, if you keep the button pressed until the end of the dispense cycle (when the motor stops) the reset takes place after you release the **START** button again.

 Also, you can abort the cycle (and purge) by pressing one of the mode buttons.

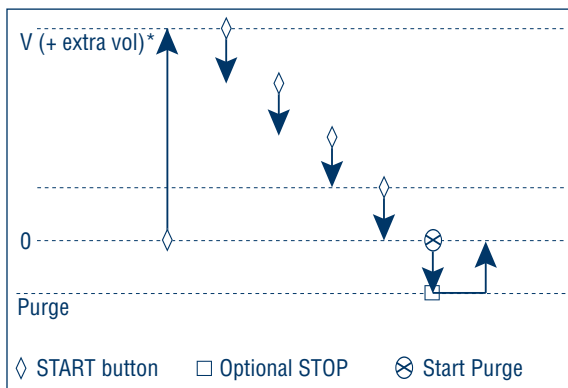

 * the needed volume plus an automatically selected excess volume.

REVERSE

a) Description:



This mode is like reverse mode pipetting using a manual pipette and recommended for viscous liquid. Please refer to the Gilson Guide to Pipetting for further information.

b) Protocol:

- i) Set the sample volume: turn the thumbwheel until you see the selected volume displayed on the screen, then press the thumbwheel to lock the volume – you cannot dispense until this is done.
- ii) Set the speed (optional): press the +/- keys to increase or reduce the speed (default is 5). The speed can be changed before or during a pipetting cycle.

c) Functionality:

- i) Immerse the tip in the liquid to be aspirated.
- ii) To aspirate*: press the **START** button, wait until the motor resets and stops at the end of the aspiration phase.
- iii) To dispense: press and release the **START** button.
- iv) "BLOW OUT" appears on the screen: click on **START** to purge and reset the piston. However, if you keep the button pressed until the end of the dispense cycle (when the motor stops) the reset takes place after you release the **START** button again.

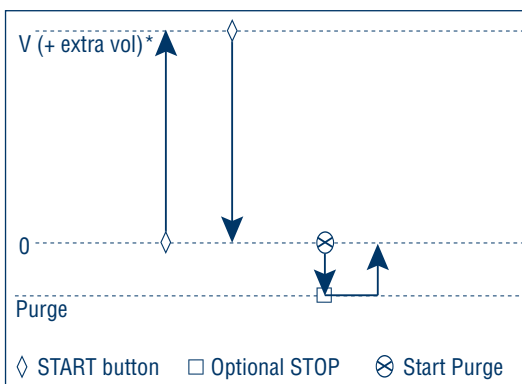

* the needed volume plus an automatically selected excess volume.

Also, you can abort the cycle (and purge) by pressing one of the Mode buttons in every modes.

The REVERSE mode may be replaced by a pre-programmed mode uploaded from your computer (see below).

Programming Modes

You may replace REVERSE with your own custom built mode, which you have programmed on a Personal Computer (PC) with the Pipetman Concept Utility Software. You have total flexibility and an almost unlimited number of combinations are possible (see program guide).

To operate in the program mode, you need a PC and a kit (reference F30755) containing the necessary software and connectors. The kit is available from your usual Gilson distributor (see Chapter 15).

Typically you can do the following and combine protocol tasks at will:

DILUTE

Aspirate volumes V1 and V2 with an air gap between the two volumes then distribute the ensemble.

DILUTE AND MIX

Aspirate volumes V1 and V2 with an air gap between the two volumes, mix (as above), then distribute the mixture.

MULTIPLE ASPIRATES

Aspirate N times a volume and then distribute the ensemble.

DISTRIBUTION WITH TIMER


Distribute multiple aliquots with a user defined time interval between each.

7 GILSON DIAMOND TIPS

Gilson Diamond Tips are made to the highest specifications, strict quality control is maintained throughout the manufacturing process.

Diamond Tips are used to calibrate Pipetman Concept, therefore for optimum performance, you are strongly advised to use Gilson's Diamond Tips with your Pipetman Concept. Diamond Tips have the Gilson logo engraved on their collar, ensuring that you have a genuine Gilson product. To ensure accuracy and precision, Gilson's Quality Assurance System focuses on the following critical parameters.

- Diamond Tips are made from pure polypropylene (virgin, metal-free, to avoid the possibility of contamination). They are available sterilized and with filters.

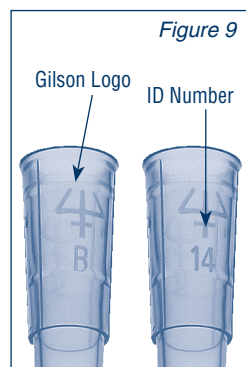

- Gilson's sterilized Diamond Tips are certified free of detectable RNases, DNases, DNA, RNA, and proteases.
- Optimized shape (revised collar for optimum sealing, thin walls, and fine point), making them easier to mount, more flexible, with no vortexing, and improved precision.
- Diamond Tips are free from defects, especially at the orifice. All surfaces are smooth and hydrophobic, thereby avoiding the excessive retention of liquids that causes poor accuracy and a lack of precision.
- Mold and cavity references are marked on the collar, ensuring the traceability for quality assurance purposes, batch numbers appear on all packages (bags and boxes).
- They form an air-tight seal with the tip-holder, preventing the leaks that cause poor accuracy and a lack of precision.
- They may be autoclaved at 121°C for 20 minutes at 0.1 MPa.

8 PIPETTING TECHNIQUES

Guidelines for Good Pipetting

- 1) Make sure that you fit new tips.
- 2) Each new tip(s) should be pre-rinsed with the liquid to be pipetted.
- 3) When aspirating, keep the tip(s) at a constant depth below the surface of the liquid (refer to Table 1).
- 4) Change the tip(s) before aspirating a different liquid, sample, or reagent.
- 5) Change the tip(s) if a droplet remains at the end of the tip(s) from the previous pipetting operation.
- 6) Liquid should never enter the tip holder. To prevent this:
 - Never turn the pipette upside down,
 - Never lay the pipette on its side when there is liquid in the tip(s),
 - Refer to the specific mode for details of the functionality.
- 7) The use of the Gilson Charging Stand (see Chapter 15) is recommended to store your Pipetman Concept pipette in the vertical position.
- 8) When pipetting liquids with temperatures different to the ambient temperature, pre-rinse the tip(s) several times before use in order to reach an equilibrium between the temperatures of the liquid and the pipette's air-cushion.
- 9) For volatile liquids you should saturate the aircushion of your pipette by aspirating and dispensing the liquid repeatedly before aspirating the sample.

- 10) After pipetting acids or other corrosive liquids that emit vapors, clean the pipette, as described in Chapter 12.
- 11) The pipette can be used between + 4 °C and + 40 °C, but the specifications may vary.
- 12) Do not pipette liquids having temperatures above 70°C or below 4°C.



Extreme temperatures can affect accuracy and precision.

Aspirate and Dispense

- 1) Fit new Gilson Diamond Tip(s) (for the best results - see “Specifications”, Chapter 17). Push the tip-holder into the tip using a slight twisting motion to ensure a firm and airtight seal.

- 2) Pre-rinse the tip(s).

Pre-rinsing consists of aspirating the first volume of liquid and then dispensing it back into the same vessel (or to waste). Subsequent volumes that you pipette will have levels of accuracy and precision within specifications.

Some liquids (e.g. protein-containing solutions and organic solvents) can leave a film of liquid on the inside the wall of the tip; pre-rinsing the tip minimizes any errors that may be related to this phenomenon.

- 3) Hold the pipette vertically and immerse the tip(s) in the liquid (see Table 1).

Press START to aspirate the set volume of liquid. Wait a few seconds (time depends on model, see Table 1); then withdraw the pipette-tip from the liquid.

You may wipe any droplets away from the outside of the tip(s) using a medical wipe, however if you do so **take care to avoid touching the tip’s orifice.**

Table 1 - Immersion Depth and Wait Time

Model	Immersion Depth (mm)	Wait Time (Seconds)
C10, 8x10, 12x10	1	1
C100, 8x100, 12x100	2-4	1
C300, 8x300, 12x300	2-4	1
C1200,	2-4	2-3
C5000	3-6	4-5
C10ml	5-7	4-5

- 4) Place the end of the tip(s) against the inside wall of the recipient vessel (at an angle of 10° to 40°). Press the START button. Wait for at least a few seconds before releasing the START button to expel any residual liquid from the tip(s). While removing the pipette draw the tip along the inside surface of the vessel.
- 5) Eject the tip(s) by pressing firmly on the tip ejector button.

9 GLP FEATURES

Your Pipetman Concept is fully compliant to ISO8655 standard and is CE marked (for IVD and EMC directives).

Pipetman Concept enables error-free manipulations, and includes the following GLP features.

General

- Lockable volume.
- Name of model is marked on the color-coded START button.
- Volume range is displayed on the screen and on the ejector-cover (Multichannel models).
- Serial number is engraved on the handle of the pipette and encoded in the firmware.
- Bar code: on the box and with the certificate (can be transferred).
- Personalization by nametag (for marking application or user name) and by encoding in the firmware. The name appears on the screen when the pipette goes to standby (after 3 minutes of inactivity).
- System menu can be locked from a PC thanks to the Utility Software (see Chapter 10).

Cycle counters

- From last volume setting, counts the number of cycles in the current 'run' (0 to 999). Appears on the main screen.
- From manufacture and since the last service (see Chapter 10).
- Indicators (R1, R2, R3 ... Rx) each time pipette is readjusted (see Chapters 10 & 17).
- Maintenance intervals can be specified by weeks or number of cycles elapsed. These and other parameters may be locked by the using the Pipetman Concept Utility Software.

Alarms

- Low battery warning (flashes in the place of the volume indicator).
Push any button and the message disappears – this gives a few minutes of use enabling you to finish the current manipulation and then to recharge the battery (or replace with another charged battery).
- Volume out of specifications warning (for Program mode).
- Service is overdue warnings (see Chapter 10).
- Beeper can be set On or Off.

10 SYSTEM MENU

Press **both Mode buttons** at the same time to accede to the System Menu. This menu lets you choose between 4 sub-menus: Configuration, Calibration, Maintenance and Personalization.



Select a menu by rotating the thumbwheel, then click on the required item to enter the sub-menu; select an item from the sub-menu in the same way.



You can modify the parameters associated with each one, provided that the sub-menu was not locked by computer-based software (using the PC Connection Kit, see Chapter 15).

Configuration

This menu allows you to configure the following items.

Beeper:

Click on the thumbwheel to set the beeper ON or OFF (the beeper will not operate, except in the case of an error or if set in Program mode).

Screen contrast:

Click on the thumbwheel, rotate the thumbwheel to select a value from 1 to 5, then click again to confirm the value.

Volume limit:

Click on the thumbwheel, rotate the thumbwheel to select a volume (default = nominal), then click again to confirm the value.

To return to the currently active screen: select Quit and click to confirm.

```
> Configuration*
Calibration
Maintenance
Personalization
Quit
```

PIPETMAN Concept

* asterisk means that the system menu is locked.

```
> Configuration
Calibration
Maintenance
Personalization
Quit
```

PIPETMAN Concept

```
> Beeper: OFF
Contrast: 3
Volume limit: 300.0
Quit
```

PIPETMAN Concept


Calibration


As part of your quality system you may have standard operating procedures for pipette calibration. In accordance with ISO 8655 Gilson recommends a gravimetric procedure for pipette calibration. Please refer to “Verification Procedure for Accuracy and Precision, reference LT802292”, which you can download from the Gilson website.

This gravimetric method is used to establish the mean mass of a given volume of water (taking into account evaporation losses, where necessary). After converting the mean mass to a volume (using the Z factor), you enter the measured volumes(s) into the pipettes memory and the software readjusts the pipette accordingly.

Pipetman Concept allows the user to adjust the pipette quickly with maximum accuracy and with the flexibility to use one, three or four calibration points (see below).

The calibration menu allows you to access the following items: Standard Readjustment, Quick Re-adjustment or Factory setting.

 *Following readjustment by the user, R_n (R_1 , R_2 , etc) is displayed on the active screen to indicate the number of times the pipette has been readjusted since manufacture. The value of n is increased by 1 when you use Quit to leave the screen after a modification or confirmation of the values.*

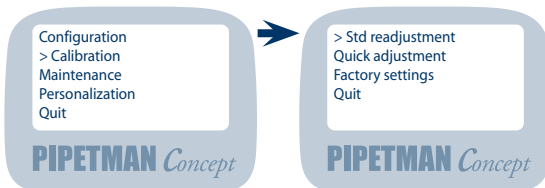


You select the operation that you wish to perform using the thumbwheel, and then click the thumbwheel to access the corresponding parameters. After this, select the volume that you wish to enter, click the thumbwheel, turn the thumbwheel until you see the measured volume, and click to confirm the value.

Continue this process for the other volumes (if any), then select Quit and click to confirm.


Standard Readjustment


This menu allows you to readjust the pipette using 3 calibration points: 10 %, 50 % and 100 % of nominal volume nominal (according the recommendation of ISO8655). These three values are stored in the firmware.

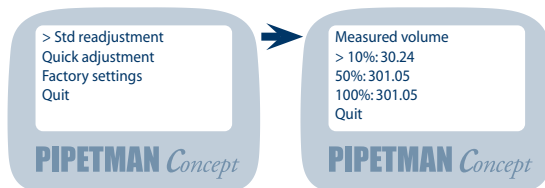

Quick Adjustment

This menu allows you to adjust the pipette using 1 calibration point. Effectively, by adding a fourth point to the standard calibration values. By default the value stored in the firmware is zero in which case it is not taking into account as a fourth calibration point.

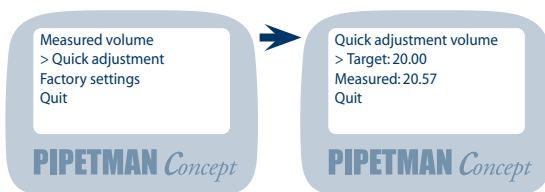

 If the value entered for Calibration volume is the same as one of the values used for the Standard re-adjustment then the Measured volume of Quick readjustment will replace the Measured volume of Standard readjustment when calculating the correction to be used.

Factory Settings

This option allows you to reset the volumes to the three factory calibration values (Std. Adjustment), which are permanently stored in the pipette's firmware.

 If you choose this option you will erase the fourth calibration point from the Quick Readjustment procedure.

Maintenance


This menu allows you to check and set parameters relating to pipette maintenance. Select a sub-menu by rotating the thumbwheel, then click on the required item to enter the sub-menu; select an item from the sub-menu in the same way. Routine maintenance procedures are described in the next Chapter.

Disassembly



This option allows you to disassemble the lower part safely (protection of the piston and the motor). If you select "Disassembly", the following screen appears:

To close the "Disassembly" menu, the only possibility is to choose "Quit".

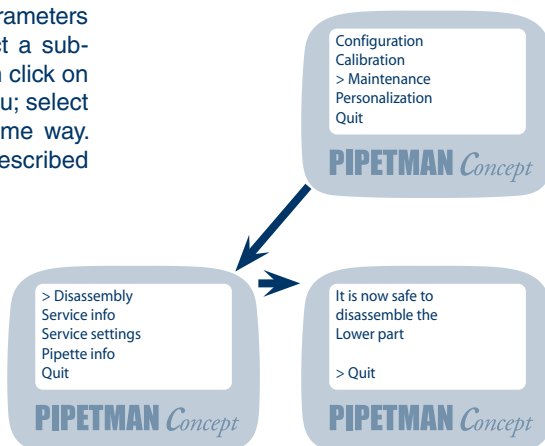


If you select "Quit", a confirmation message appears. If you select "No", the display will return to the "Disassembly" menu. If you select "Yes", **you must first ensure that the pipette has been correctly reassembled** (see Chapter 11). The software then resets the piston and the display returns to the last mode used.

PIPETMAN *Concept*[®]

Service Info

This screen is **read only** – you cannot modify any of the items, which are: the number of cycles and the date since the pipette was serviced.






Service Settings

Select an item by rotating the thumbwheel, then click on the required item to select it; rotate the thumbwheel to select a value (e.g. “Weeks”) and then click on the thumbwheel to confirm.

You can change four variables: “Cycles” to next service, “Weeks” to next service, “Date” of the service, and “Alarm” (see below).

When it comes to setting the date, you have three fields to modify, one after the other, day - month - year (dd mm yy) in the same way as the other parameters mentioned above.

 The 3 letters for the months are as follows; JAN, FEB, MAR, APR, MAY, JUN, JUL, SEP, OCT, NOV, DEC.





Maintenance Alarm

By default the maintenance alarm is set to OFF – rotating the thumbwheel alternates between On and Off confirm by pressing the thumbwheel. Warning messages will be displayed depending on the maintenance settings that you make (see Chapter 11).

Pipette info

This screen is **read only** – you cannot modify any of the items, which are:


- The serial number of the pipette.
- The version of the firmware.
- The number of cycles since the pipette was manufactured.



Personalization

This menu allows you to personalize the standby screen.

Select “New Id”. With the cursor aligned as shown (>A), click and turn the thumbwheel to select a character and click it to confirm. You may enter a string of up to 15 alphanumeric characters. Use the asterisk (*) to signal that you have entered the last character; use / to cancel.



11 USER MAINTENANCE

It is best to inspect your pipette regularly and to routinely clean and change parts if required. To help you to keep up a regular schedule and in the interests of GLP, you can configure your pipette to display an alarm before a service is due (refer to Chapter 10). Setting maintenance alarm to “On” results in the following messages.

Maintenance Warnings

- Date of next service: warning about 1 week before and if overdue.
- If you exceed a service interval that was set relative to the number of pipetting cycles, the system flashes the following message place of the volume indicator.

Push any button and the following is displayed.

Select “Maintenance ?” to go to the system menu or “Remind me later” to delay by one day.


- If you exceed a service interval that was set relative to a time limit, the system flashes the following message place of the volume indicator.

Select “Maintenance ?” to go to the system menu or “Remind me later” to delay by one day.

Maintenance Operations

You may perform the following operations yourself.

- Clean or autoclave the parts specified under “Cleaning and Decontamination”, Chapter 12
- Change the parts specified under “Replacement Parts”, Chapter 15
- Lubricate the piston,
- Change the battery.

 Please contact your Gilson distributor if you require their assistance in the form of training or if you would like to enter into a service contract with them.



Go to Maintenance>Disassembly and confirm to disassemble the lower part safely (see page 21).

Cycles: 20000
> Weeks: 36
Date: 18 JAN 07
Alarm: ON
Quit

PIPETMAN Concept

SERVICE PIPETTE NOW!
[Time limit passed]

> Maintenance ?
Remind me later

PIPETMAN Concept


Maintenance Operations for Single-channel models

Tip-holder and Tip-ejector

These parts must be changed, if they are accidentally damaged or attacked chemically. You should also remove these parts for cleaning or decontamination purposes.

Changing the Tip-ejector




- 1) Keep the tip-ejector button depressed, and grip the top of the tip-ejector with the other hand.
- 2) Gently rotate the tip-ejector counterclockwise and separate its connector from the activating rod (figure 10).
- 3) Pull the tip-ejector away from the handle of the pipette.
- 4) Clean or autoclave the tip-ejector and refit it (or a new one) by reversing the procedure.

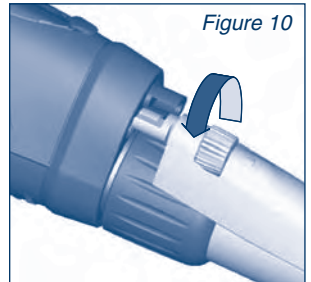

Changing the Tip-holder (lower part)

After removing the tip-ejector, you may remove the lower part of the tip-holder, which is more likely to become contaminated or damaged than the upper part. Removal of the lower part is shown below; for the upper part refer to “Removing the Piston” (special precautions are necessary).

- 1) Gently rotate the lower part of the tip-holder counterclockwise to unscrew it from the upper part (figure 11).
- 2) Separate the parts and remove the O-ring (see “Changing the O-ring”, figures 12 and 13).
- 3) Clean and if required autoclave the lower part of the tip-holder.
- 4) If required lubricate the piston (see “How to Lubricate the Piston”) and fit a new O-ring.
- 5) Screw the two parts together; making sure that the two parts are fully tightened by hand, using latex gloves.
- 6) Refit the tip-ejector.

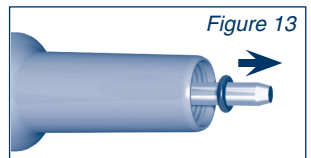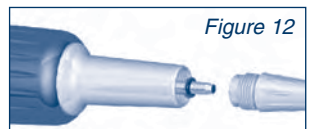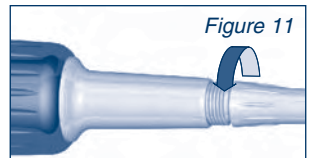

Changing the O-ring (or seal for C10)

The O-ring is contained by the two halves of the tip-holder; if worn or damaged in any way, it must be replaced.

To access the O-ring, remove the tip-ejector and unscrew the lower part of the tip-holder - if the O-ring is not immediately visible on the piston, select the AUTO mode then set the volume to the nominal and press the ACTION button. You should now be able to remove the O-ring from the piston. Sometimes, the O-ring may be found in the recess at the top-end of the lower part of the tip-holder.

If required lubricate the piston (see “How to Lubricate the Piston”) then fit a new O-ring by sliding it onto the piston. Reassemble the pipette.

Servicing the Piston


 You may remove the piston-assembly to clean, lubricate, or change the piston.

The specifications of the pipette must be checked after changing the piston.

Removing the Piston

 **Use the stand-by procedure (Disassembly, see Chapter 10: “Maintenance”).**

- 1) Select the “Disassembly” option in the System menu (System menu>Maintenance>Disassembly).
- 2) Remove the tip-ejector and (optionally) the lower part of the tip-holder. If you remove the lower part, take care to remove the piston seal as described in “Changing the O-ring”.
- 3) Unscrew the connecting-nut (turn by hand, counterclockwise, figure 14).
- 4) Pull on the spring guide to remove the piston assembly from the handle of the pipette - separate the parts (figure 15). For C5000 and C10 ml, the connecting nut is combined with the upper part of the tip-holder (see “Spare Parts”).
- 5) Clean and autoclave (if required) the piston and holder, together with any other parts that may need to be treated in the same way (see “Cleaning and Decontamination”).
- 6) Lubricate the piston (except C10), see at the end of chapter.
- 7) Reassemble the piston, spring and spring guide; then carefully insert the assembly into the handle of the pipette (figure 16). The spring guide should hold the piston assembly inside the handle of the pipette.

 **Take care to position the small-diameter end of the spring as shown (innermost), and that the flanged end of the spring guide is outermost.**

- 8) Reassemble the upper part of the tip-holder and the connecting nut, and then refit to the handle of the pipette by rotating the connecting nut clockwise until it is finger tight (figure 17). Fit the seal and reassemble the lower part of the tip-holder. Refit the tip ejector.

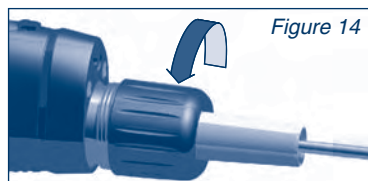


Figure 14

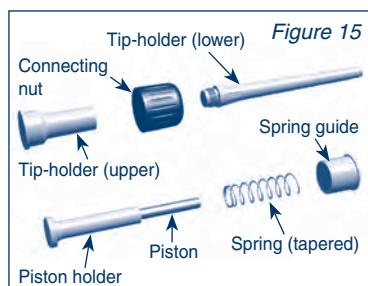


Figure 15

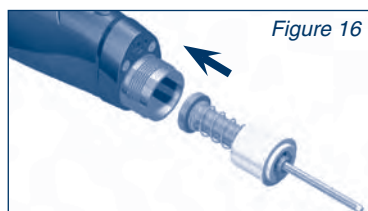


Figure 16

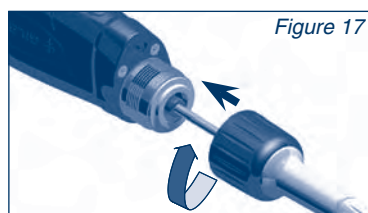



Figure 17

 The seal for C10 is fragile and can only be used once. So, after unscrewing the lower part of the tip-holder you must fit a new seal.

- Quit the “Disassembly” screen (Quit>Yes).

Maintenance Operations for Multichannel models

Removing and reassembling the Head

 **Use the stand-by procedure (Disassembly, see Chapter 10: “Maintenance”).**

- Select the “Disassembly” option in the System menu (System menu>Maintenance>Disassembly).
- Keep the tip-ejector button depressed and grip the ejector-clip.
- Unlock the ejector-clip and separate it from the activating rod (figure 18).
- Unscrew the connecting nut.
- Extract the head.
- After reassembling the head, quit the “Disassembly” screen (Quit>Yes).

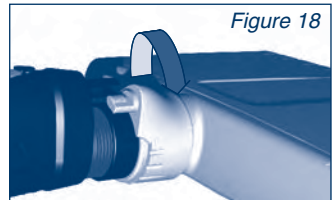


Figure 18

Removing the Plastic Cover, Piston Assemblies and Tip-holders

- Remove the two screws, which are located at either side of the head, using a miniature screwdriver (figure 19).
- Gently pull the ejector-cover away from the head (figure 20).
- Remove the wire clips (+ wire guides for 12 channels-models) from the piston tray-cover (figure 21).
- Lay the pipette flat and push awards (with your thumbs) on the catches at either side of the piston-tray cover (figure 22). The cover will flip upwards to reveal piston and tip-holder assemblies.
- Lift the tip-holder upwards, away from the lower rake, then push the tip-holder back along the axis of the piston.




Figure 19




Figure 20

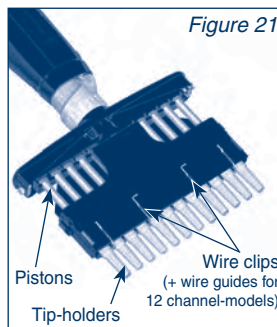


Figure 21

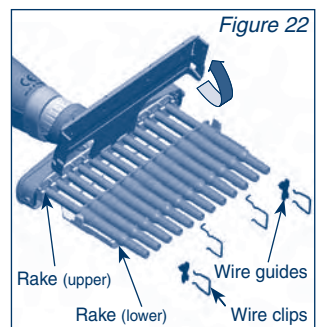


Figure 22

Now, pull the piston away from the upper rake and lift it and the tip holder out of the tray, taking care not to lose or damage the piston spring.


- 6) Gently pull the piston assembly out of the tip-holder.

Servicing the Ejector-cover, Piston Assemblies and Tip-holders (all models except Multichannel x10)

The tip-holders and piston assemblies must be changed, if they are accidentally damaged or attacked chemically (figures 23 and 24).

You should also remove them for cleaning or decontamination purposes, and to lubricate the pistons.

- 1) Examine the ejector-cover, if it is cracked or badly corroded it should be replaced with a new part. Otherwise, it should be cleaned and if necessary autoclaved.
- 2) Check the piston for damage or corrosion. Lubricate and replace as necessary.
- 3) After removing the locking clip, gently pry out each tip-holder's internal components: locking-clip, spring, O-ring and seal-holder (figure 25) – this can be done using the reassembly tool. Replace or clean and decontaminate these components. Replace or clean and decontaminate the tip-holder.





 *The O-ring can get trapped in tip-holder. Use a fine plastic probe to extract the O-ring.*

Reassembling the Piston Assemblies, Tip-holders, and Plastic Ejector-cover

A) Tip-holders

- 1) Use a lubricated piston to transfer a small quantity of lubricant to the O-ring.
- 2) With reference to the figure 26, place the components on the reassembly tool in the following order: locking-clip, tip-holder spring, seal-holder, O-ring – take care that the spring is the correct way up and the flat surface of seals, rings and washers faces the spring.
- 3) Insert the components into the tip-holder with the aid of the reassembly tool.
- 4) Push on the locking-clip until it snaps into place.

Tip-holder 8x300/12x300

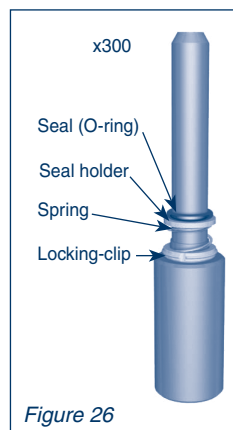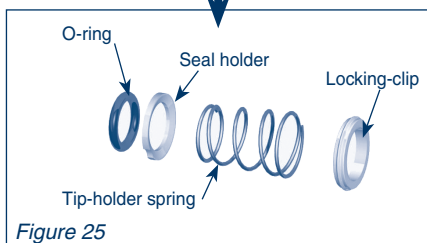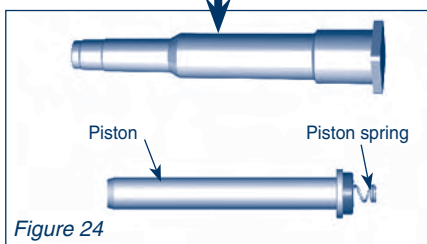

B) Piston Assemblies

- 1) Lubricate the piston, as described in the section below.
- 2) Gently, slip a lubricated piston into the tip-holder, with a slight twisting motion. Avoid using too much force as this could dislodge the O-ring.

C) Closing-up

- 1) Refit each tip-holder/piston assembly so that the top of the piston and the tip-holder snap into the upper and lower rakes, respectively. To facilitate fitting a piston assembly to the upper rake, you should incline the piston assembly and compress the piston-spring against the upper rake, before pushing the assembly into place.
- 2) Close the piston tray-cover, after checking that all assemblies are correctly installed.
- 3) Refit the wire-clips (+ wire guides for 12 channel-models).
- 4) Slide the ejector-cover back over the piston-tray and reattach using the two screws.

How to Lubricate the Piston (all models, except C10 and Multichannel x10)

Use only Gilson lubricant (ref: F3070902, as supplied). Squeeze a small quantity from the tube onto a clean, nonabrasive cloth. Use the cloth to transfer the lubricant to the piston. Ensure that the piston is evenly lubricated, and that you wipe away any excess - remember only a fine film of lubricant is required (over the entire piston).

12

CLEANING AND DECONTAMINATION

Pipetman Concept is designed so that the parts normally in contact with liquid contaminants can easily be cleaned and decontaminated.

As part of your quality system, you may have procedures for pipette decontamination. We recommend that you refer to “Decontamination Procedures for Gilson Pipettes” (reference LT802288), which you can download from Gilson’s website.



Liquid must not enter the handle of the pipette.

If you use chemical solutions for decontamination or detergents for cleaning, other than specified below, you should check with your supplier that the solution or detergent used does not attack any of the following materials: stainless steel, POM (Polyoxymethylene), PVDF (Polyvinylidene fluoride), PC (Polycarbonate) and PBT (Polybutylene Terephthalate).

Cleaning

The pipette must be cleaned, as described below, before it is decontaminated. You may use a simple soap solution for cleaning Pipetman Concept or any of the solutions mentioned in “Decontamination Procedures for Gilson Pipettes” (reference LT802288).

External

- 1) Remove the tip-ejector (see Chapter 11).
- 2) Wipe the tip-ejector with a soft-cloth or lint-free tissue impregnated with soap solution.
- 3) Wipe the entire pipette with a soft-cloth or lint-free tissue impregnated with soap solution, to remove all dirty marks. If the pipette is very dirty, a brush with soft plastic bristles may be used.
- 4) Wipe the entire pipette and the tip-ejector with a soft cloth or lint-free tissue impregnated with distilled water.

Internal

The following components only can be immersed in a cleaning solution: tip-ejector, tip-holder (both parts), connecting nut, piston (including holder), return spring, and spring guide.

- 1) Disassemble the pipette as described in Chapter 11.
- 2) Set aside the upper part in a dry and secure location.
- 3) Clean the individual components of the lower part of the pipette using an ultrasonic bath (20 minutes at 50°C) or with a soft-cloth and brushes. Small round brushes with soft plastic bristles may be used to clean the interior of the tip-holder.
- 4) Rinse the individual components with distilled water.
- 5) Leave the parts to dry by evaporation or wipe them with a clean soft-cloth or lint-free tissue.
- 6) Lubricate the piston and reassemble the pipette according to the instructions given earlier in the previous chapter.

Decontamination

Autoclaving

The handle of the pipette is not autoclavable. Only the following parts may be autoclaved individually: tip-ejector, tip-holder (both parts), connecting nut, piston (including holder), return spring, spring guide, O-ring (warning: can be damaged when autoclaved), and airtightness kit (Multichannel models).

- 1) Clean the parts to be autoclaved, especially the tip-holder.
- 2) Put the parts in an autoclaving sack.
- 3) Autoclave at 0.1 MPa at 121°C for 20 minutes.
- 4) Check that the parts are dry before reassembling the pipette.
- 5) Set the pipette aside to stabilize at room temperature.



The specifications of the pipette must be checked after autoclaving.

Chemical Decontamination

You may choose to decontaminate your pipette chemically, in accordance with your own procedures. Whatever decontaminant you use, check that it is compatible with the plastics used in the construction of the pipette (see previous page).

- Parts that may not be immersed
 - 1) Wipe the handle of the pipette with a soft-cloth or lint-free tissue impregnated with the chosen decontaminant.
 - 2) Wipe the handle of the pipette with a soft-cloth or lint-free tissue impregnated with distilled water.

- Parts that may be immersed

The following components only can be immersed in a decontaminant solution: tip-ejector, tip-holder (both parts), connecting nut, piston (including holder), return spring, and spring guide.

- 1) Disassemble the pipette as described in "Maintenance".
- 2) Immerse the components in the decontaminant solution or wipe them according the instructions given by the manufacturer or supplier of the decontaminant.
- 3) Rinse the individual components with distilled or sterile water.
- 4) Leave the parts to dry by evaporation or wipe them with a clean lint-free tissue or soft-cloth.
- 5) Lubricate the piston and reassemble the pipette according to the instructions given in this chapter.

13 LEAK TEST

This test may be performed at any time to check that the pipette does not leak, especially after performing a maintenance or decontamination procedure. If a pipette fails this test you should replace the O-ring and seal and repeat this test, after making sure that the pipette is correctly reassembled.

C10 to C300 Single and Multichannel

- fit a Gilson Diamond Tip,
- set the pipette to the maximum volume given in the specifications, and pre-rinse,
- aspirate the set volume from a beaker of distilled water,
- maintain the pipette in the vertical position and wait for 20 seconds,
- if a water droplet appears at the end of the tip there is a leak,

- if you see no droplet, re-immers the tip below the surface of water,
- the water level inside the tip should remain constant; if the level goes down there is a leak.

C1200 to C10ml

- fit a Gilson Diamond tip,
- set the pipette to the maximum volume given in the specifications,
- aspirate the set volume from a beaker of distilled water,
- maintain the pipette in the vertical position and wait for 20 seconds,
- if a water droplet appears at the end of the tip, there is a leak.

14 TROUBLESHOOTING

In case of malfunction, first press the reset button located in the back of the pipette between the power supply and the PC connector. Insert a small plastic probe (like a tip) in the hole and press. If the problem persists, you may consult the following table which identifies potential problems and their solutions.



Before returning any pipette to your local Gilson Service Center, ensure that it is completely free of chemical, biological, or radioactive contamination. Please use the included safety bag.

Symptom	Possible Cause	Refer to page
Pipette is leaking sample	Worn O-ring	23-24, 26
Pipette won't aspirate	Worn O-ring	23-24, 26
	Unscrewed lower part of tip holder	23
	Damaged or corroded piston	24-26
	Damaged tip holder	23, 25-27
	Improper repair or assembly	22-27
	Connecting nut is loose	25
Noisy operation	Piston needs lubricating	27
Pipette is inaccurate	Improper repair or assembly	22-27
	Unscrewed lower part of tip-holder	23
	Pipette is out of adjustment	18-20
	Connecting nut is loose	25
Pipette is not precise	Unscrewed lower part of tip-holder	23
	Incorrect operator technique	15-16
	Worn O-ring	23-24, 26
	Connecting nut is loose	25
	Damaged or corroded piston	24-26
	Damaged tip-holder	23, 25-27
Tips fall off or don't fit	Low quality tips	14-15
	Damaged tip-holder	23, 25-27
	Damaged tip-ejector	24-26
No LCD display	Pipette is not switched on	7
	Battery needs recharging	4

15 ACCESSORIES & REPLACEMENT PARTS

Accessories

Item	Reference
Rapid Charging Stand	F30750
PC Connection Kit (including Pipetman Concept Utility Software)	F30755
Pipetman Concept Utility Software	F3075502
Name Tag	F3071107
AC-adapter Europe	F30701
AC-adapter USA/Japan	F30702
AC-adapter UK	F30703
AC-adapter Australia	F30704

Replacement Parts for Pipetman Concept Single channel

Item		C10	C100	C300	C1200	C5000	C10ml
Battery block	①	F3071165	F3071165	F3071165	F3071165	F3071165	F3071165
Adjustable hook	②	F3071110	F3071110	F3071110	F3071110	F3071110	F3071110
Personalization window	③	F3071103	F3071103	F3071103	F3071103	F3071103	F3071103
Tip ejector assembly	④	F2070159	F2070459	F2070559	F2070659	F2070759	F2070859
Piston assembly	⑤	F3071252	F3071352	F3071452	F3071552	F3071652	F3071752
Return spring	⑥	F2070113	F2070113	F2070113	F2070113	-	-
Spring guide	⑦	F307115451	F307115451	F307115451	F307115451	-	-
Tip holder, upper part	⑧	F2070117	F2070417	F307145302	F2070617	-	-
O-ring, x 5 (or seal for C10)	⑨	F161902	F2070401	F307145351	F2070601	F2070701	F2070801
Tip holder, lower part	⑩	F2070218	F2070418	F307145301	F2070618	F2070719	F2070819
Connecting nut	⑪	F2072111	F2072111	F2072111	F2072111	-	-
Tip ejector extension for C10		F2070903	-	-	-	-	-
Lubricant tube 3.5 g		-	F3070902	F3070902	F3070902	F3070902	F3070902
Bag of 10 filters		-	-	-	-	F161280	F161280
Bag of 100 filters		-	-	-	-	F161240	F161240

Replacement Parts for Pipetman Concept Multichannel

Item		8x10	8x100	8x300	12x10	12x100	12x300
Battery block	①	F3071165	F3071165	F3071165	F3071165	F3071165	F3071165
Adjustable hook	②	F3071110	F3071110	F3071110	F3071110	F3071110	F3071110
Personal. window	③	F3071103	F3071103	F3071103	F3071103	F3071103	F3071103
Screws and wire clips kit	⑫	F2073261	F2073261	F2073261	F2073361	F2073361	F2073361
Tip holder assembly G-F.I.T. system	⑬	F3073255	F3073355	F307326306	F3073255	F3073355	F307326306
Ejector cover	⑭	F307325051	F307335051	F2073259	F307425051	F307435051	F2073359
Piston assembly	⑮	F3073254	F3073354	F3073454	F3073254	F3073354	F3073454
Air tightness kit	⑯	-	F3073360	F2073265	-	F3073360	F2073265
Reassembly tool		F3073201	F3073301	F2073201	F3073201	F3073301	F2073201
Lubricant tube 3.5 g		-	F3070902	F3070902	F3070902	F3070902	F3070902

16 SAFETY PRECAUTIONS AND LIMITATIONS OF USE

For safety reasons, it is important to observe the following instructions:

1- Battery and electrical specifications

- We strongly recommend you fully charge the battery before using the pipette.
- Your Gilson distributor supplies an AC adaptor that is suitable for your country - either in the pipette box or separately. You must only use an original Gilson AC adaptor specific to this product. Charge the battery in the pipette, using the AC-adaptor or the charging stand, or in the charging stand (slot for additional battery).
- Use AC-adaptor and charging stand indoors.
- When handling the battery, do not allow the battery to come into contact with any metallic surfaces. Do not short circuit.
- Dispose of used batteries in accordance with legal regulations. Batteries may not be disposed of with household waste and may explode if disposed in fire !
 - Li-ion battery pack; 1 Ah / 3.6 V
Charging time: approx. 2 hours for a fully discharged battery (80% in one hour).
⚠ Symbol means: Caution, risk of danger.
 - AC adaptor (may be not included; see above)
Input voltage, country-specific: 100-240 V, 50/60 Hz (0.5A max.)
Output voltage: +5 V DC; 3.5A (17.5W max.)

2- Do not use Pipetman Concept in a potentially explosive environment

or with potentially explosive chemicals.

3- When pipetting infectious, radioactive, toxic and other hazardous solutions,

please observe all the safety precautions (e.g. wear protective clothing, goggles and gloves) and regulations appropriate for your country.

4- Do not allow the liquid to enter the body of the pipette.**5- Storage conditions**

Temperature: -20°C to 50°C

Humidity max: 80%

6- Temperature of use

Between 4°C and 40°C (specifications may vary).

7- Use only original Gilson's Diamond tips, accessories and spare parts.

If the equipment is used in a manner not specified by Gilson in the user's guide, the protection provided in the equipment may be impaired.

8- Equipment disposal

This equipment must not be disposed of with unsorted municipal waste. Instead, it is your responsibility to correctly dispose of your waste equipment by handing it over to an authorised facility for separate collection and recycling. It is also your responsibility to decontaminate the equipment in case of biological, chemical, and/or radiological contamination so as to protect from health hazards the persons involved in the disposal and recycling of equipment.

For more information about where you can drop off your waste equipment for recycling, please contact your local dealer from whom you originally purchased the product or your local council.

By doing so, you will help conserve natural resources and you will ensure that your waste equipment is recycled in a manner that protects human health and the environment. Thank you!

17 SPECIFICATIONS

Pipetman Concept is a high quality pipette that offers excellent accuracy and precision. The figures given in the “Gilson Maximum Permissible Errors” table were obtained using mode AUTO (speed 5). These figures are only guaranteed using Genuine Gilson Diamond Tips.

Each pipette is inspected and validated by qualified technicians according to the Gilson Quality System.

Gilson declares that its manufactured pipettes comply with the requirements of the ISO 8655 Standard, by type testing. The adjustment is carried out under strictly defined and monitored conditions (ISO 8655-6):


- Basis of adjustment, Ex.
- Reference temperature, 20 °C
- Relative humidity, 50 %
- Barometric pressure, 101 kPa
- Use of distilled water grade 3 (ISO 3696)
- Ten measurements for each test volume, which are Nominal Volume, 50 % of Nominal Volume, and 10% of Nominal Volume.

18 GILSON MAXIMUM PERMISSIBLE ERRORS

Tested mode: AUTO. Speed: 5.

The data conform to ISO 8655-2 Standard.

Model/Color coding (Reference) Range	Diamond Tips*	Volume (μ L)	Gilson		ISO 8655	
			Systematic error (μ L)	Random error (μ L)	Systematic error (μ L)	Random error (μ L)
C10/Red (F31012) 0.5 - 10 μ L	D10 DL10	0.5	± 0.040	≤ 0.013	± 0.120	≤ 0.080
		1	± 0.025	≤ 0.012	± 0.120	≤ 0.080
		5	± 0.060	≤ 0.020	± 0.120	≤ 0.080
		10	± 0.080	≤ 0.025	± 0.120	≤ 0.080
C100/Peach (F31013) 5 - 100 μ L	D200	5	± 0.35	≤ 0.10	± 0.80	≤ 0.30
		10	± 0.30	≤ 0.10	± 0.80	≤ 0.30
		50	± 0.38	≤ 0.12	± 0.80	≤ 0.30
		100	± 0.40	≤ 0.15	± 0.80	≤ 0.30
C300/Green (F31014) 20 - 300 μ L	D300	20	± 0.80	≤ 0.16	± 4.00	≤ 1.50
		30	± 0.70	≤ 0.20	± 4.00	≤ 1.50
		150	± 0.90	≤ 0.23	± 4.00	≤ 1.50
		300	± 1.05	≤ 0.30	± 4.00	≤ 1.50
C1200/Blue (F31015) 100 - 1200 μ L	D1200	100	± 2.5	≤ 0.4	± 16.0	≤ 6.0
		120	± 2.4	≤ 0.4	± 16.0	≤ 6.0
		600	± 3.6	≤ 0.8	± 16.0	≤ 6.0
		1200	± 6.0	≤ 1.2	± 16.0	≤ 6.0
C5000/Purple (F31016) 500 - 5000 μ L	D5000	500	± 10	≤ 2	± 40	≤ 15
		2500	± 15	≤ 4	± 40	≤ 15
		5000	± 25	≤ 7	± 40	≤ 15
C10ml/Light blue (F31017) 1 - 10mL	D10ml	1 mL	± 25	≤ 4	± 60	≤ 30
		5 mL	± 30	≤ 8	± 60	≤ 30
		10 mL	± 50	≤ 12	± 60	≤ 30
8x10 - 12x10/Red (F31032) - (F31042) 0.5 - 10 μ L	DL10	1	± 0.04	≤ 0.02	± 0.24	≤ 0.16
		5	± 0.08	≤ 0.04	± 0.24	≤ 0.16
		10	± 0.10	≤ 0.06	± 0.24	≤ 0.16
8x100 - 12x100/Peach (F31033) - (F31043) 5 - 100 μ L	D200	10	± 0.25	≤ 0.14	± 1.60	≤ 0.60
		50	± 0.50	≤ 0.20	± 1.60	≤ 0.60
		100	± 0.80	≤ 0.25	± 1.60	≤ 0.60
8x300 - 12x300/Green (F31034) - (F31044) 20 - 300 μ L	D300	30	± 1.0	≤ 0.18	± 8.0	≤ 3.0
		150	± 1.5	≤ 0.38	± 8.0	≤ 3.0
		300	± 2.4	≤ 0.60	± 8.0	≤ 3.0

 * Recommended tip for establishing maximum permissible errors (ISO 8655 requirement).
A large range of suitable Gilson Diamond tip is available.

Please contact your local Gilson distributor for further information.

EC DECLARATION OF CONFORMITY

The company,

GILSON S.A.S.

19, avenue des Entrepreneurs
BP. 145 - 95400 Villiers-le-Bel (France)
Tel.: +33(0)1 34 29 50 00
Fax: +33(0) 1 34 29 50 20

Hereby certifies on its sole responsibility that the products listed below:

Pipetman Concept[®]

C10, C100, C300, C1200, C5000, C10ml,
8x10, 8x100, 8x300,
12x10, 12x100x 12x300

*comply with the requirements of
the following European Directives:*

98/79/EC*
on In Vitro Diagnostic
Medical Devices

89/336/EEC
Electromagnetic Compatibility, EMC

** Annex III, self-declared*

Villiers-le-Bel, September 14th, 2005



Atika El Sayed
General Manager



Hervé Ledorze
Quality Manager



NOTES

LT801489/C - ©2007 Gilson SAS All rights reserved
English

June 2007
Printed in France



World Headquarters

Gilson, Inc.

3000 Parmenter Street, P. O. Box 620027, Middleton, WI 53562-0027, USA
Telephone: (1) 800-445-7661 or (1) 608-836-1551 Fax: (1) 608-831-4451

Gilson SAS

19 avenue des Entrepreneurs, B. P. 145, 95400 Villiers-le-Bel, France
Telephone: (33) 1-34-29-50-00 Fax: (33) 1-34-29-50-20